

# FOOD SAFETY & ENVIRONMENTAL PRODUCT CATALOG














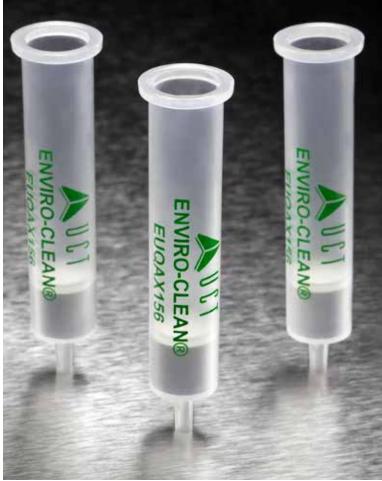











Founded in 1986, UCT has grown to be a respected leader in the drug testing, pharmaceutical, clinical, environmental and agricultural industries. Our wide range of highly reproducible solid-phase extraction columns allow the chromatographer a consistent extraction technique, and our expertise in silane manufacturing allows greater control of the chemical processes involved in producing our high quality bonded phases. We manufacture our complete product line of bonded silica sorbents, packaged in a variety of formats, including SPE columns, 96 & 48 well plates, Universal cartridges and micro-centrifuge tubes. We also offer a variety of SPE accessories including derivatizing reagents, GC liners, and manifolds. Recently we launched several new product lines: Selectra® HPLC columns, Ultra Flash® Purification, and SpinFiltr™. Our commitment to ensuring the satisfaction of our customers is accomplished by delivering on our promises: top-quality, dependable solid-phase extraction and chromatography products, and unmatched technical support.



# A GREENER EARTH


Here at UCT, Inc. we are making an effort to keep the planet cleaner and greener for everyone. It is our belief that we must act now to preserve our environment for future generations to come.

Organizations we support:
Arbor Day Foundation
Audubon Society
Sierra Club



# **TABLE OF CONTENTS**

QuECHERS Multi-Packs - Mylar Pouches + Centrifuge Tubes       .06         QuECHERS Multi-Packs - Mylar Pouches + Centrifuge Tubes       .06         Mylar Pouches - Standalone       .07         Centrifuge Tube Format       .08         Dispersive SPE (dSPE) Clean-up Sorbents       .09         2 ml dSPE Format       .09         15 ml dSPE Format       .09         16 ml dSPE Format       .09         15 ml dSPE Format       .09         16 ml dSPE Format       .09         15 ml dSPE Format       .09         16 ml dSPE Format       .00         Mylar Pouches + Centrifuge Tubes       .11         Mylar Pouches - Centrifuge Tubes       .11         ChloroFiltr*       .12         Spring Tube       .12         Quick QueChers       .13         LipiFiltr*       .13         LipiFiltr*       .14         Ouick QueChers       .15         SPE Cartridge Clean-up       .17         ENVIRO-CLEAN* Universal and Specialty Cartridges       .18         ENVIRO-CLEAN* Universal Cartridges       .18         ENVIRO-CLEAN* Public Cartridges       .18         ENVIRO-CLEAN* Public Cartridges       .24         ENVIRO-CLEAN* Selication Cartridges <t< th=""><th>QuEChERS Line</th><th></th></t<>	QuEChERS Line	
Mylar Pouches - Standalone.       07         Centrifuge Tube Format - Salts pre-loaded.       08         Dispersive SPE (dSPE) Clean-up Sorbents.       09         2 ml dSPE Format.       10         Multi-Pack - Mylar Pouches + Centrifuge Tubes.       11         Mylar Pouches - Standalone.       11         ChloroFiltr**       12         SpinFiltr*       13         LipiFiltr*       14-15         Ouick QuEChERS.       16         SPE Cartridge Clean-up.       17         ENVIRO-CLEAN* Universal and Specialty Cartridges       18-23         ENVIRO-CLEAN* Universal Cartridges       19         ENVIRO-CLEAN* Specialty Cartridges       20         ENVIRO-CLEAN* Specialty Cartridges       20         ENVIRO-CLEAN* Specialty Cartridges       20         ENVIRO-CLEAN* Specialty Cartridges       22         ENVIRO-CLEAN* Specialty Cartridges       24-25         ENVIRO-CLEAN* Specialty Cartridges       24-25         ENVIRO-CLEAN* Glyphosate Purification Cartridges       24-25         ENVIRO-CLEAN* Fusion* Ag*       26-29         ENVIRO-CLEAN* Fusion* Ag*       26-29         ENVIRO-CLEAN* Fusion* Ag*       26-29         ENVIRO-CLEAN* Solid-Phase Extraction Cartridges       37	QuEChERS Extraction Salts	06
Centrifuge Tube Format - Salts pre-loaded         .08           Dispersive SPE (dSPE) Clean-up Sorbents         .09           2 ml dSPE Format         .09           15 ml dSPE Format         .09           Multi-Pack - Mylar Pouches + Centrifuge Tubes         .11           Mylar Pouches - Standalone         .11           Mylar Pouches - Standalone         .12           SpinFiltr®         .13           LipFiltrB         .13           Quick QuEChERS         .14           Specartidge Clean-up         .17           ENVIRO-CLEAN® Universal and Specialty Cartridges         .18-           ENVIRO-CLEAN® Universal and Specialty Cartridges         .19           ENVIRO-CLEAN® Specialty Cartridges         .20           ENVIRO-CLEAN® Specialty Cartridges         .20           ENVIRO-CLEAN® HL DVB         .20           ENVIRO-CLEAN® Bulk Cartridges         .24           ENVIRO-CLEAN® Glyphosate Purification Cartridges         .24           ENVIRO-CLEAN® Glyphosate Purification Cartridges         .24           ENVIRO-CLEAN® Fusion® Ag*         .26           ENVIRO-CLEAN® Fusion® Ag*         .26           ENVIRO-CLEAN® Fusion® Ag*         .26           ENVIRO-CLEAN® Solid-Phase Extraction Cartridges         .33		
Dispersive SPE (dSPE) Clean-up Sorbents.       .09         2 ml dSPE Format.       .09         15 ml dSPE Format.       .10         Multi-Pack - Mylar Pouches + Centrifuge Tubes.       .11         Mylar Pouches - Standalone.       .11         ChloroFiltr**       .12         SpinFiltr**       .13         LipiFiltr**       .14         Quick QuEChERS.       .14         SPE Cartridge Clean-up.       .17         ENVIRO-CLEAN** Universal and Specialty Cartridges       .19         ENVIRO-CLEAN** Specialty Cartridges.       .19         ENVIRO-CLEAN* Push-Through Cartridges.       .20         ENVIRO-CLEAN* Push-Through Cartridges.       .20         ENVIRO-CLEAN* Push-Through Cartridges.       .24         ENVIRO-CLEAN* Glyphosate Purification Cartridges.       .24         ENVIRO-CLEAN* Fusion* Ag*       .26         ENVIRO-CLEAN* Fusion* Ag*       .27         ENVIRO-CLEAN* Solid-Phase Extraction Cartridges.       .27         ENVIRO-CLEAN* Solid-Phase Extraction Cartridges.       .27         ENVIRO-CLEAN* Solid-Phases.       .30         .1       .4         Copolymeric Phases.       .4         .1       .4         Copolymeric Phases.       .4	Mylar Pouches - Standalone	07
2 ml dSPE Format		
15 ml dSPE Format		
Multi-Pack - Mylar Pouches + Centrifuge Tubes       .11         Mylar Pouches - Standalone       .11         ChloroFiltre*       .12         SpinFiltre*       .13         LuipFiltre*       .14-15         Ouick QuEChERS       .16         SPE Cartridge Clean-up       .17         ENVIRO-CLEAN® Universal and Specialty Cartridges       .19         ENVIRO-CLEAN® Universal Cartridges       .19         ENVIRO-CLEAN® Specialty Cartridges       .20         ENVIRO-CLEAN® Specialty Cartridges       .20         ENVIRO-CLEAN® Specialty Cartridges       .20         ENVIRO-CLEAN® Specialty Cartridges       .20         ENVIRO-CLEAN® Specialty Cartridges       .24-25         ENVIRO-CLEAN® Push-Through Cartridges       .24-25         ENVIRO-CLEAN® Fusion® Ag*       .26-29         ENVIRO-CLEAN® Fusion® Ag* Cartridges       .27         ENVIRO-CLEAN® Fusion® Ag* Cartridges       .27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       .30-51         Hydrophobic Phases       .33         Hydrophilic Phases       .37         Anion-Exchange Phases       .40         Cation-Exchange Phases       .40         Cation-Exchange Phases       .44         Copolymeric Phases		
Mylar Pouches - Standalone		
ChloroFiltr®       .12         SpinFiltr®       .13         LipiFiltr®       .14-15         Quick QuEChERS       .16         SPE Cartridge Clean-up       .17         ENVIRO-CLEAN® Universal and Specialty Cartridges       .19         ENVIRO-CLEAN® Universal Cartridges       .19         ENVIRO-CLEAN® Specialty Cartridges       .20         ENVIRO-CLEAN® Specialty Cartridges       .20         ENVIRO-CLEAN® 8270       .22         ENVIRO-CLEAN® 8270       .22         ENVIRO-CLEAN® Push-Through Cartridges       .24-25         ENVIRO-CLEAN® Glyphosate Purification Cartridges       .24         ENVIRO-CLEAN® Fusion® Ag* Cartridges       .27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       .30-51         Hydrophilic Phases       .33         Hydrophilic Phases       .33         Hydrophilic Phases       .40         Cation-Exchange Phases       .40         Cation-Exchange Phases       .40         Copolymeric Phases       .45         Polymeric Phases       .45         Polymeric Phases       .50         Inert Glass Cartridge       .51         ENVIRO-CLEAN® Bulk Sorbent       .52         Salation Vacuum Manifold <td< td=""><td></td><td></td></td<>		
SpinFiltr®		
LipiFiltr®       14-15         Quick QuEChERS       16         SPE Cartridge Clean-up       17         ENVIRO-CLEAN® Universal and Specialty Cartridges       18-23         ENVIRO-CLEAN® Universal Cartridges       20         ENVIRO-CLEAN® Specialty Cartridges       20         ENVIRO-CLEAN® 8270       22         ENVIRO-CLEAN® 8270       22         ENVIRO-CLEAN® Glyphosate Purification Cartridges       24-25         ENVIRO-CLEAN® Glyphosate Purification Cartridges       24         ENVIRO-CLEAN® Fusion® Ag+       26-29         ENVIRO-CLEAN® Fusion® Ag+ Cartridges       27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       30-51         Hydrophobic Phases       33         Hydrophobic Phases       33         Anion-Exchange Phases       40         Cation-Exchange Phases       40         Cation-Exchange Phases       45         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       55         6 Station Vacuum Manifold       55         SELECTRA® U/HPLC Columns       58-61         SELECTRA® C18		
Quirk QuEChERS       16         SPE Cartridge Clean-up       17         ENVIRO-CLEAN® Universal and Specialty Cartridges       19         ENVIRO-CLEAN® Universal Cartridges       19         ENVIRO-CLEAN® Specialty Cartridges       20         ENVIRO-CLEAN® HL DVB       20         ENVIRO-CLEAN® Push-Through Cartridges       24-25         ENVIRO-CLEAN® Push-Through Cartridges       24-25         ENVIRO-CLEAN® Fusion® Ag+       26-29         ENVIRO-CLEAN® Fusion® Ag+       26-29         ENVIRO-CLEAN® Fusion® Ag+ Cartridges       27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       30-51         Hydrophobic Phases       33         Hydropholic Phases       37         Anion-Exchange Phases       44         Cation-Exchange Phases       44         Copolymeric Phases       44         Copolymeric Phases       45         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       58         SELECTRA® U/HPLC Columns       58-61         SELECTRA® Aqueous C18       60	·	
SPE Cartridge Clean-up       .17         ENVIRO-CLEAN® Universal Cartridges       .18-23         ENVIRO-CLEAN® Universal Cartridges       .19         ENVIRO-CLEAN® Specialty Cartridges       .20         ENVIRO-CLEAN® HL DVB       .20         ENVIRO-CLEAN® 8270       .22         ENVIRO-CLEAN® Push-Through Cartridges       .24-25         ENVIRO-CLEAN® Glyphosate Purification Cartridges       .24         ENVIRO-CLEAN® Fusion® Ag+       .26-29         ENVIRO-CLEAN® Fusion® Ag+ Cartridges       .27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       .30-51         Hydrophobic Phases       .33         Hydrophobic Phases       .33         Anion-Exchange Phases       .40         Cation-Exchange Phases       .44         Cation-Exchange Phases       .45         Polymeric Phases       .50         Inert Glass Cartridge       .51         ENVIRO-CLEAN® Bulk Sorbent Guide       .52-53         ENVIRO-CLEAN® Bulk Sorbent Guide       .55         ENVIRO-CLEAN® Bulk Sorbent       .56         SELECTRA® U/HPLC Columns       .58-61         SELECTRA® U/HPLC Columns       .58-61         SELECTRA® Aqueous C18       .60         SELECTRA® Aqueous C18       .60		
ENVIRO-CLEAN* Universal and Specialty Cartridges   18-23		
19	SECULTINGE Clean-up	17
19	ENVIRO-CLEAN® Universal and Specialty Cartridges	18-23
ENVIRO-CLEAN® Specialty Cartridges       20         ENVIRO-CLEAN® 10 DVB       20         ENVIRO-CLEAN® 8270       22         ENVIRO-CLEAN® 10 Push-Through Cartridges       24-25         ENVIRO-CLEAN® Glyphosate Purification Cartridges       24         ENVIRO-CLEAN® Fusion® Ag+       26-29         ENVIRO-CLEAN® Fusion® Ag+ Cartridges       27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       30-51         Hydrophobic Phases       33         Hydropholilic Phases       37         Anion-Exchange Phases       40         Cation-Exchange Phases       45         Polymeric Phases       45         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® DA       59         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® Aqueous C18       60         SELECTRA® C8       61         Accessories       62-66         GC Liner		
ENVIRO-CLEAN® HL DVB       20         ENVIRO-CLEAN® 8270       22         ENVIRO-CLEAN® Push-Through Cartridges       24-25         ENVIRO-CLEAN® Glyphosate Purification Cartridges       24         ENVIRO-CLEAN® Fusion® Ag+       26-29         ENVIRO-CLEAN® Fusion® Ag+ Cartridges       27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       30-51         Hydrophobic Phases       33         Hydrophobic Phases       37         Anion-Exchange Phases       40         Cation-Exchange Phases       45         Polymeric Phases       45         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       62-66         Reservoirs       64-65		
ENVIRO-CLEAN® 8270		
ENVIRO-CLEAN® Push-Through Cartridges         24-25           ENVIRO-CLEAN® Glyphosate Purification Cartridges         24           ENVIRO-CLEAN® Fusion® Ag+         26-29           ENVIRO-CLEAN® Fusion® Ag+ Cartridges         27           ENVIRO-CLEAN® Solid-Phase Extraction Cartridges         30-51           Hydrophobic Phases         33           Hydrophilic Phases         37           Anion-Exchange Phases         40           Cation-Exchange Phases         44           Copolymeric Phases         45           Polymeric Phases         50           Inert Glass Cartridge         51           ENVIRO-CLEAN® Bulk Sorbent Guide         52-53           ENVIRO-CLEAN® Bulk Sorbent         53           Manifolds         54-57           Glass Block Vacuum Manifold         55           Glass Block Vacuum Manifold         55           SELECTRA® DA         59           SELECTRA® C18         60           SELECTRA® Apepous C18         60           SELECTRA® PFPP         61           SELECTRA® C8         61           Accessories         62-66           GC Liners         63           Reservoirs         64-65		
ENVIRO-CLEAN® Glyphosate Purification Cartridges       24         ENVIRO-CLEAN® Fusion® Ag+       26-29         ENVIRO-CLEAN® Fusion® Ag+ Cartridges       27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       30-51         Hydrophobic Phases       33         Hydrophilic Phases       37         Anion-Exchange Phases       40         Cation-Exchange Phases       45         Copolymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       62-66         GC Liners       63         Reservoirs       64-65	LIVINO CLEAN 0270	
ENVIRO-CLEAN® Glyphosate Purification Cartridges       24         ENVIRO-CLEAN® Fusion® Ag+       26-29         ENVIRO-CLEAN® Fusion® Ag+ Cartridges       27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       30-51         Hydrophobic Phases       33         Hydrophilic Phases       37         Anion-Exchange Phases       40         Cation-Exchange Phases       45         Copolymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       62-66         GC Liners       63         Reservoirs       64-65	ENVIRO-CLEAN® Push-Through Cartridges	24-25
ENVIRO-CLEAN® Fusion® Ag+       26-29         ENVIRO-CLEAN® Fusion® Ag+ Cartridges       27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       30-51         Hydrophobic Phases       33         Hydrophilic Phases       47         Anion-Exchange Phases       40         Cation-Exchange Phases       44         Copolymeric Phases       45         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       55         SELECTRA® DA       59         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65		
ENVIRO-CLEAN® Fusion® Ag+ Cartridges       27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       30-51         Hydrophobic Phases       33         Hydrophilic Phases       37         Anion-Exchange Phases       40         Cation-Exchange Phases       44         Copolymeric Phases       50         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® DA       59         SELECTRA® DA       59         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65	Zivinio GZZi iv Gippiloodio i dimoddon odi ilagoominii ilanii ila	
ENVIRO-CLEAN® Fusion® Ag+ Cartridges       27         ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       30-51         Hydrophobic Phases       33         Hydrophilic Phases       37         Anion-Exchange Phases       40         Cation-Exchange Phases       44         Copolymeric Phases       50         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® DA       59         SELECTRA® DA       59         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65	ENVIRO-CLEAN® Fusion® Aq+	26-29
ENVIRO-CLEAN® Solid-Phase Extraction Cartridges       30-51         Hydrophobic Phases       33         Hydrophilic Phases       37         Anion-Exchange Phases       40         Cation-Exchange Phases       44         Copolymeric Phases       45         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       55         SELECTRA® U/HPLC Columns       58-61         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65		
Hydrophobic Phases       33         Hydrophilic Phases       37         Anion-Exchange Phases       40         Cation-Exchange Phases       45         Copolymeric Phases       45         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® Reperp       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65		
Hydrophobic Phases       33         Hydrophilic Phases       37         Anion-Exchange Phases       40         Cation-Exchange Phases       45         Copolymeric Phases       45         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® Reperp       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65	ENVIRO-CLEAN® Solid-Phase Extraction Cartridges	30-51
Anion-Exchange Phases       40         Cation-Exchange Phases       44         Copolymeric Phases       45         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65		
Cation-Exchange Phases       44         Copolymeric Phases       45         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65		
Copolymeric Phases       45         Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® DA       59         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® FPPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65	Anion-Exchange Phases	40
Polymeric Phases       50         Inert Glass Cartridge       51         ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® DA       59         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65	Cation-Exchange Phases	44
Inert Glass Cartridge	Copolymeric Phases	45
ENVIRO-CLEAN® Bulk Sorbent Guide       52-53         ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65	Polymeric Phases	50
ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65	Inert Glass Cartridge	51
ENVIRO-CLEAN® Bulk Sorbent       53         Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65		
Manifolds       54-57         6 Station Vacuum Manifold       55         Glass Block Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® DA       59         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65		
6 Station Vacuum Manifold	ENVIRO-CLEAN® Bulk Sorbent	53
6 Station Vacuum Manifold		
Glass Block Vacuum Manifold       57         SELECTRA® U/HPLC Columns       58-61         SELECTRA® DA       59         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65	Manifolds	54-57
SELECTRA® U/HPLC Columns       58-61         SELECTRA® DA       59         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65		
SELECTRA® DA       59         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65	Glass Block Vacuum Manifold	57
SELECTRA® DA       59         SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65		
SELECTRA® C18       60         SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65		
SELECTRA® Aqueous C18       60         SELECTRA® PFPP       61         SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65		
SELECTRA® PFP       61         SELECTRA® C8       62         Accessories       62         GC Liners       63         Reservoirs       64-65		
SELECTRA® C8       61         Accessories       62-66         GC Liners       63         Reservoirs       64-65	SELECTRA® Aqueous C18	60
Accessories       62-66         GC Liners       63         Reservoirs       64-65		
GC Liners	SELECTRA C8	61
GC Liners	Accessing	00.00
Reservoirs64-65		
FIIIS		
	FIIIS	
Customer Service	Customer Service	67

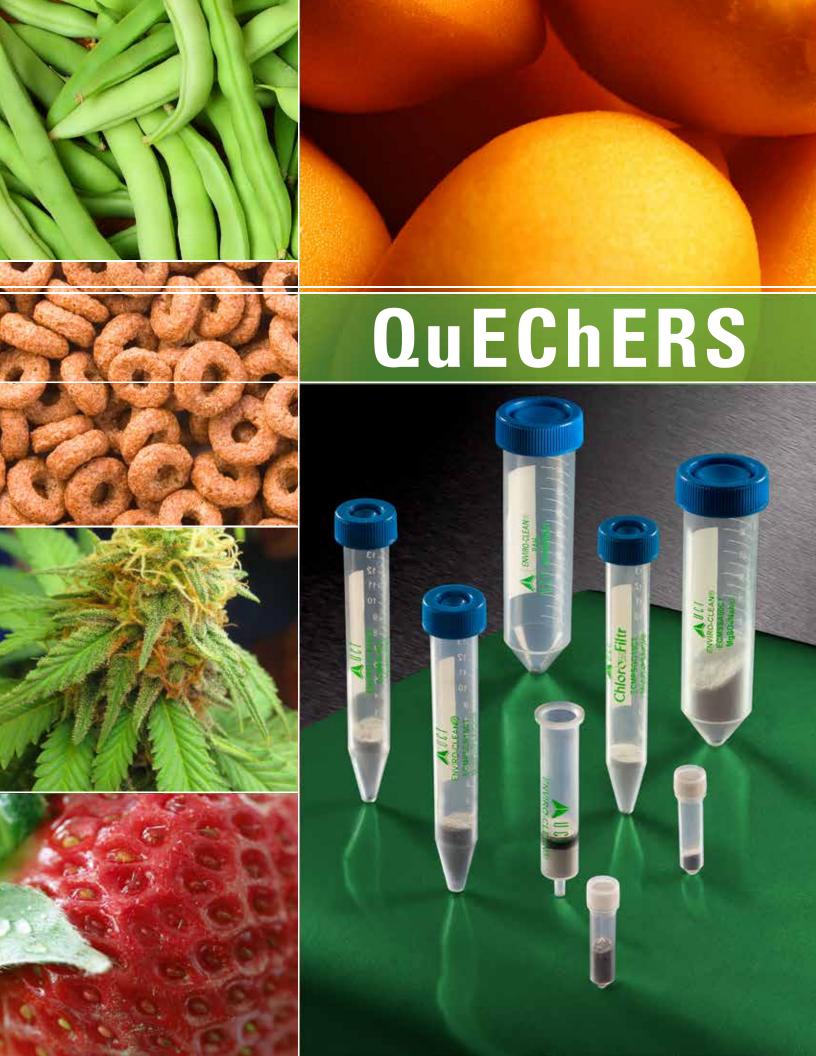

# **QuEChERS Methods Schematic Flow Chart**

# Original QuEChERS Anastassiades and Lehotay 2003

#### Unbuffered

Add 10 mL of ACN to 10 g homogenized/hydrated sample in a 50 mL centrifuge tube Add ISTD Shake



Add 4 g MgSO<sub>4</sub> & 1 g NaCl Shake vigorously for 1 minute Centrifuge at > 3000 rcf for 1 minute

(ECMSSC50CT-MP)

#### Step 1 - Extraction Processes

#### AOAC QuEChERS AOAC 2007.01

#### **Acetate Buffered**

Add 15 mL of 1% HOAc in ACN to
15 ml homogenized/hydrated sample in
a 50 mL centrifuge tube
Add ISTD
Shake



Add 6 g MgSO<sub>4</sub> & 1.5 g NaOAc Shake vigorously for 1 minute Centrifuge at >3000 rcf for 1 minute

(ECMSSA50CT-MP)

#### CEN QuECHERS EN 15662

#### Citrate Buffered

Add 10 mL of ACN to 10 g homogenized/hydrated sample in a 50 mL centrifuge tube Add ISTD Shake



Add 4 g MgSO<sub>4</sub>, 1 g NaCl, 1 g Na<sub>3</sub>Citrate·2H<sub>2</sub>O, 0.5 g Na2HCitr·1.5H<sub>2</sub>O Shake vigorously for 1 minute Centrifuge at >3000 rcf for 1 minute

(ECQUEU750CT-MP)

Step 2 - Dispersive SPE Clean-Up Processes



Transfer 1 mL aliquot of supernatant to a dSPE clean-up tube containing 150 mg MgSO<sub>4</sub> and 50 mg

Shake for 30 seconds

Centrifuge at > 1500 rcf for 1 minute

(CUMPS2CT)



Transfer 0.5 mL to vial for GC or LC analysis



Transfer 1 mL aliquot of supernatant to a dSPE clean-up tube containing MgSO<sub>4</sub>, PSA (C18, GCB or ChloroFiltr can be added for additional clean-up)

Shake for 30 seconds

Centrifuge at > 1500 rcf for 1 minute

(CUMPS2CT)
OR
(CUMPS2C1875CB2CT)



Preserve with toluene for GC/MS or

add 6.7mM formic acid for LC/MS/MS

Add TPP surrogate



Transfer 1 mL aliquot of supernatant to a dSPE clean-up tube containing 25 mg of PSA and 150 mg MgSO<sub>4</sub>, (plus 2.5 or 7.5 mg of GCB to remove pigments)

Shake for 30 seconds

Centrifuge at > 1500 rcf for 1 minute

(ECQUEU32CT) OR (ECQUEU42CT)



Preserve with 5% formic acid in ACN.

Analyze by GC/MS or LC/MS/MS

MgSO<sub>4</sub>-magnesium sulfate

ACN-acetonitrile

HoAC-acetic acid

NaCl-sodium chloride

Na<sub>3</sub>Citr.-sodium citrate tribasic dihydrate

Na<sub>3</sub>HCitr.-sodium citrate dibasic sesquihydrate

PSA-primary secondary amine

TPP-triphenyl phosphate (surrogate)

GCB-graphitized carbon black

#### **Extraction Components and Their Functions**

MgSO, - Facilitates solvent partitioning

ACN - Provides the extraction of broadest range of pesticides with least amount of undesired matrix

HoAC - Adjusts pH

Buffer Salts - Prevent degredation of pH sensitive analytes

PSA - Removes sugars, acids, and some pigments

GCB - Strong sorbent for pigment removal

C18 - Removes long-chain fatty compounds and other non-polar interferences

# Multi-Packs - Mylar Pouches + Centrifuge Tubes

QuEChERS extraction salts for all of the popular QuEChERS methods are available in individual mylar pouches for your convenience. Each pack of 50 pouches comes with a rack of 50 empty centrifuge tubes.



Part Number	Description	Quantity	Contents
ECMSSC50CT-MP	Non-Buffered Extraction	50/Pack	4000 mg MgSO₄ 1000 mg NaCl
ECQUUS250CT-MP	Non-Buffered Extraction	50/Pack	4000 mg MgSO₄ 2000 mg NaCl
ECMSSC50CTFS-MP	Non-Buffered Extraction	50/Pack	6000 mg MgSO₄ 1500 mg NaCl
EC4MSSA50CT-MP	AOAC 2007.01 Method	50/Pack	4000 mg MgSO₄ 1000 mg NaOAc
ECMSSA50CT-MP	AOAC 2007.01 Method	50/Pack	6000 mg MgSO₄ 1500 mg NaOAc
ECQUEU750CT-MP	EN 15662 Method	50/Pack	4000 mg MgSO <sub>4</sub> 1000 mg NaCl 500 mg Na <sub>2</sub> HCitr.1.5H <sub>2</sub> O 1000 mg Na <sub>3</sub> Citr.2H <sub>2</sub> O
ECMIV50CT-MP	EN 15662 Method	50/Pack	6000 mg MgSO <sub>4</sub> 1500 mg NaCl 750 mg Na <sub>2</sub> HCitr.1.5H <sub>2</sub> O 1500 mg Na <sub>3</sub> Citr.2H <sub>2</sub> O
ECQUUS950CT-MP	THC Potency & Pesticides	50/Pack	Proprietary Salt Blend for THC Potency & Pesticide Testing

# **Mylar Pouch Format**











Part Number	Description	Quantity	Contents
ECMSSC-MP	Non-Buffered Extraction	50/Pack	4000 mg MgSO₄ 1000 mg NaCl
ECQUUS2-MP	Non-Buffered Extraction	50/Pack	4000 mg MgSO₄ 2000 mg NaCl
ECMSSCFS-MP	Non-Buffered Extraction	50/Pack	6000 mg MgSO₄ 1500 mg NaCl
ECQUVIN-MP	Non-Buffered Extraction	50/Pack	8000 mg MgSO <sub>4</sub> 2000 mg NaCl
EC4MSSA-MP	AOAC 2007.01 Method	50/Pack	4000 mg MgSO <sub>4</sub> 1000 mg NaOAc
ECMSSA-MP	AOAC 2007.01 Method	50/Pack	6000 mg MgSO₄ 1500 mg NaOAc
ECGMSSA-MP	AOAC 2007.01 Method	50/Pack	6000 mg MgSO <sub>4</sub> (granular) 1500 mg NaOAc
ECQUEU7-MP	EN 15662 Method	50/Pack	4000 mg MgSO <sub>4</sub> 1000 mg NaCl 500 mg Na <sub>2</sub> HCitr.1.5H <sub>2</sub> O 1000 mg Na <sub>3</sub> Citr.2H <sub>2</sub> O
ECGQUEU7-MP	EN 15662 Method	50/Pack	4000 mg MgSO <sub>4</sub> (granular) 1000 mg NaCl 500 mg Na <sub>2</sub> HCitr.1.5H <sub>2</sub> O 1000 mg Na <sub>3</sub> Citr.2H <sub>2</sub> O
ECMIV-MP	EN 15662 Method	50/Pack	6000 mg MgSO <sub>4</sub> 1500 mg NaCl 750 mg Na <sub>2</sub> HCitr.1.5H <sub>2</sub> O 1500 mg Na <sub>3</sub> Citr.2H <sub>2</sub> O

# **QuEChERS Extraction Salts**

# **Centrifuge Tube Format**

UCT offers an extensive selection of QuEChERS extraction salts pre-packed in either 15 or 50 ml polypropylene centrifuge tubes.



Part Number	Description	Volume	Quantity	Contents
ECMS4MSC550CT	Non-Buffered Extraction	50 mL	50/Pack	4000 mg MgSO₄ 500 mg NaCl
ECMSSC50CT	Non-Buffered Extraction	50 mL	50/Pack	4000 mg MgSO₄ 1000 mg NaCl
ECMSSC50CTFS	Non-Buffered Extraction	50 mL	50/Pack	6000 mg MgSO₄ 1500 mg NaCl
ECQUVIN50CT	Non-Buffered Extraction	50 mL	50/Pack	8000 mg MgSO₄ 2000 mg NaCl
ECMS4MSA1M50CT	AOAC 2007.01 Method	50 mL	50/Pack	4000 mg MgSO₄ 1000 mg NaOAc
ECMSSA50CT	AOAC 2007.01 Method	50 mL	50/Pack	6000 mg MgSO₄ 1500 mg NaOAc
ECQUEU750CT	EN 15662 Method	50 mL	50/Pack	4000 mg MgSO <sub>4</sub> 1000 mg NaCl 500 mg Na <sub>2</sub> HCitr.1.5H <sub>2</sub> O 1000 mg Na <sub>3</sub> Citr.2H <sub>2</sub> O
EUMIV50CT	EN 15662 Method	50 mL	50/Pack	6000 mg MgSO <sub>4</sub> 1500 mg NaCl 750 mg Na <sub>2</sub> HCitr.1.5H <sub>2</sub> O 1500 mg Na <sub>3</sub> Citr.2H <sub>2</sub> O
ECQUUS1015CT	Non-Buffered Extraction	15 mL	50/Pack	400 mg MgSO <sub>4</sub> 100 mg NaCl
ECQUUS1115CT	Non-Buffered Extraction	15 mL	50/Pack	800 mg MgSO₄ 200 mg NaCl
ECQUUS15CT	AOAC 2007.01 Method	15 mL	50/Pack	400 mg MgSO₄ 100 mg NaOAc
ECQUEU415CT	EN 15662 Method	15 mL	50/Pack	$4000 \text{ mg MgSO}_4$ $1000 \text{ mg NaCl}$ $500 \text{ mg Na}_2\text{HCitr.1.5H}_2\text{O}$ $1000 \text{ mg Na}_3\text{Citr.2H}_2\text{O}$

# Dispersive-SPE (dSPE) Sorbents



#### dSPE Clean-Up

UCT offers the most extensive line of dSPE products, conveniently packaged in centrifuge tube format. Each corresponding part number contains pre-weighed sorbents for use with Original, Association of Analytical Communities (AOAC) and European Committee for Standardization (CEN) QuEChERS methods. UCT dSPE kits make sample prep quick and easy for multi-residue analysis in a wide variety of matrices.

Part Number	Volume	Quantity	Contents
ECQUME12CT	2 mL	100/Pack	200 mg PSA
ECQUEU12CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 25 mg PSA
CUMPS2CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 50 mg PSA
ECQUEU52CT	2 mL	100/Pack	$300 \text{ mg MgSO}_4 + 50 \text{ mg PSA}$
CUMC182CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 50 mg C18
ECQUEU252CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 7.5 mg GCB
ECQUEU22CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 25 mg PSA + 25 mg C18
CUMPSC18CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 50 mg PSA + 50 mg C18
CUMPS15C18CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 150 mg PSA + 50 mg C18
ECQUEU32CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 25 mg PSA + 2.5 mg GCB
ECQUEU42CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 25 mg PSA + 7.5 mg GCB
CUMPSCB2CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 50 mg PSA + 50 mg GCB
CUMSC1875CB2CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 50 mg C18 + 7.5 mg GCB
ECQUAU12CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 25 mg Aminopropyl + 7.5 mg GCB
ECQUUS72CT	2 mL	100/Pack	50 mg PSA + 50 mg C18 + 25 mg GCB
CUMPSC1875CB2CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 50 mg PSA + 50 mg C18 + 7.5 mg GCB
ECQUEU122CT	2 mL	100/Pack	150 mg MgSO $_4$ + 50 mg PSA + 50 mg C18 + 50 mg GCB
ECQUUS142CT	2 mL	100/Pack	Proprietary Sorbent Blend for Pesticide Testing in Cannabis

<sup>\*</sup> All C18 sorbent utilized in dSPE clean-up configurations above is endcapped.

# Dispersive-SPE (dSPE) Sorbents

### 15/50 mL Format

Part Number	Volume	Quantity	Contents
EEC18515CT	15 mL	50/Pack	500 mg C18
ECQUAS815CT	15 mL	50/Pack	300 mg DVB
ECQUEU2515CT	15 mL	50/Pack	450 mg MgSO <sub>4</sub> + 450 mg C18
ECQUAS315CT	15 mL	50/Pack	750 mg MgSO <sub>4</sub> + 250 mg C18
ECQUUS515CT	15 mL	50/Pack	900 mg MgSO <sub>4</sub> + 150 mg C18
ECMPS15CT	15 mL	50/Pack	900 mg MgSO <sub>4</sub> + 150 mg PSA
ECQUAS415CT	15 mL	50/Pack	900 mg MgSO <sub>4</sub> + 300 mg PSA
ECMPSA15CT	15 mL	50/Pack	1200 mg MgSO <sub>4</sub> + 200 mg PSA
ECMS12CPSA415CT	15 mL	50/Pack	1200 mg MgSO <sub>4</sub> + 400 mg PSA
EUMPSMG15CT	15 mL	50/Pack	1500 mg MgSO <sub>4</sub> + 250 mg PSA
ECMPSA615CT	15 mL	50/Pack	1800 mg MgSO <sub>4</sub> + 600 mg PSA
ECMMCCNAX215CT	15 mL	50/Pack	1200 mg MgSO <sub>4</sub> + 200 mg Aminopropyl
ECQUEU2115CT	15 mL	50/Pack	450 mg MgSO <sub>4</sub> + 450 mg PSA + 150 mg C18
ECQUEU2415CT	15 mL	50/Pack	750 mg MgSO <sub>4</sub> + 750 mg PSA + 250 mg C18
ECQUEU315CT	15 mL	50/Pack	900 mg MgSO <sub>4</sub> + 150 mg PSA + 150 mg C18
ECMPSC1815CT	15 mL	50/Pack	900 mg $MgSO_4$ + 300 mg PSA + 150 mg C18
ECQUAS515CT	15 mL	50/Pack	900 mg MgSO <sub>4</sub> + 300 mg PSA + 300 mg C18
CUMPSC1815CT2	15 mL	50/Pack	1200 mg MgSO <sub>4</sub> + 400 mg PSA + 400 mg C18
ECQUEU515CTB	15 mL	50/Pack	885 mg $MgSO_4$ + 150 mg PSA + 15 mg GCB
ECQUEU515CT	15 mL	50/Pack	900 mg $\mathrm{MgSO_4}$ + 150 mg PSA + 15 mg GCB
ECQUEU615CT	15 mL	50/Pack	900 mg $\mathrm{MgSO_4}$ + 150 mg PSA + 45 mg GCB
ECMPSCB15CT	15 mL	50/Pack	900 mg $MgSO_4$ + 300 mg PSA + 150 mg GCB
ECQUEU1115CT	15 mL	50/Pack	1200 mg MgSO <sub>4</sub> + 400 mg PSA + 400 mg GCB
ЕСОИНКЗ15СТ	15 mL	50/Pack	700 mg MgSO <sub>4</sub> + 200 mg PSA + 200 mg C18 + 35 mg GCB
ECQUAS615CT	15 mL	50/Pack	900 mg MgSO <sub>4</sub> + 450 mg PSA + 300 mg C18 + 50 mg GCB
ECQUUS215CT	15 mL	50/Pack	1200 mg MgSO <sub>4</sub> + 400 mg PSA + 400 mg C18 + 400 mg GCB
ECC1850CT	50 mL	50/Pack	500 mg C18
ECMSC1850CT	50 mL	50/Pack	1500 mg MgSO <sub>4</sub> + 500 mg C18
ECQUUS350CT	50 mL	50/Pack	1500 mg $MgSO_4$ + 500 mg PSA + 500 mg C18

### dSPE Multi-Packs - Mylar Pouches + 15 mL Centrifuge Tubes

UCT also offers it's diverse dSPE product line in Mylar pouch format.

Part Number	Volume	Quantity	Contents
ECMPS15CT-MP	15 mL	50/Pack	900 mg MgSO <sub>4</sub> 150 mg PSA
ECMS12CPSA415CT-MP	15 mL	50/Pack	1200 mg MgSO <sub>4</sub> 400 mg PSA
ECMPSCB15CT-MP	15 mL	50/Pack	900 mg MgSO <sub>4</sub> 300 mg PSA 150 mg GCB







# Dispersive-SPE (dSPE) Sorbents

#### dSPE Mylar Pouches

Part Number	Quantity	Contents
ECMPS-MP	50/Pack	900 mg MgSO <sub>4</sub> + 150 mg PSA
ECMS12CPSA4-MP	50/Pack	1200 mg MgSO <sub>4</sub> + 400 mg PSA
ECMSC18-MP	50/Pack	1500 mg MgSO <sub>4</sub> + 500 mg C18
ECQUEU315-MP	50/Pack	900 mg MgSO <sub>4</sub> + 150 mg PSA + 150 mg C18
CUMPSC182-MP	50/Pack	1200 mg MgSO <sub>4</sub> + 400 mg PSA + 400 mg C18
ECQU001-MP	50/Pack	750 mg MgSO <sub>4</sub> + 125 mg PSA + 12.5 mg GCB
ECQU002-MP	50/Pack	750 mg MgSO <sub>4</sub> + 125 mg PSA + 37.5 mg GCB
ECQUEU5-MP	50/Pack	900 mg MgSO <sub>4</sub> + 150 mg PSA + 15 mg GCB
ECMPSCB-MP	50/Pack	900 mg MgSO <sub>4</sub> + 300 mg PSA + 150 mg GCB
ECQUEU12-MP	50/Pack	150 mg MgSO <sub>4</sub> + 50 mg PSA + 50 mg C18 + 50 mg GCB



Traditional QuEChERS methods use graphitized carbon black (GCB) to remove chlorophyll from sample extracts. Although GCB is very effective in removing chlorophyll, it can also remove planar pesticides. UCT has developed a unique sorbent that removes chlorophyll without the loss of planar pesticides. ChloroFiltr® is used as an alternative to GCB during dSPE clean-up with no method modifications needed.




Part Number	Volume	Quantity	Contents
CUMPSGG2CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 50 mg PSA + 50 mg Chlorofiltr®
ECQUCHL12CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 50 mg C18 + 50 mg Chlorofiltr®
CUMPSGGC182CT	2 mL	100/Pack	150 mg MgSO <sub>4</sub> + 50 mg PSA + 50 mg C18 + 50 mg Chlorofiltr®
ECMSGG15CT	15 mL	50/Pack	900 mg MgSO <sub>4</sub> + 150 mg Chlorofiltr®
ECMPSGG15CT	15 mL	50/Pack	900 mg MgSO <sub>4</sub> + 300 mg PSA + 150 mg Chlorofiltr®
ECQUCHL115CT	15 mL	50/Pack	900 mg MgSO <sub>4</sub> + 300 mg PSA + 300 mg Chlorofiltr®
ECQUCHL215CT	15 mL	50/Pack	900 mg MgSO <sub>4</sub> + 300 mg C18 + 300 mg Chlorofiltr®
ECQUCHL315CT	15 mL	50/Pack	900 mg MgSO <sub>4</sub> + 300 mg PSA + 300 mg C18 + 300 mg Chlorofiltr®
ECMPSGG50CT	50 mL	50/Pack	1800 mg MgSO <sub>4</sub> + 600 mg PSA + 300 mg Chlorofiltr®
ECQUCHL150CT	50 mL	50/Pack	1800 mg MgSO <sub>4</sub> + 600 mg PSA + 600 mg Chlorofiltr®
ECQUCHL250CT	50 mL	50/Pack	1800 mg MgSO <sub>4</sub> + 600 mg C18 + 600 mg Chlorofiltr®
ECQUCHL350CT	50 mL	50/Pack	1800 mg MgSO <sub>4</sub> + 600 mg PSA + 600 mg C18 + 600 mg Chlorofiltr®
WSHECQUUS14-LD	96 Well Plate Format	1	Proprietary sorbent blend for pesticide testing in cannabis



# UCT's new SpinFiltr is taking the hassle out of dSPE

- dSPE + Ultrafiltration in a single step.
- Obtain enhanced extract purification with the built-in 0.2 µm PTFE filter.
- Recover additional sample volume without worrying about the disruption of centrifugation layers.
- Simply discard dSPE chamber containing unwanted matrix and sorbet following centrifugation.

Part Number	Top Chamber Capacity	Quantity	Contents
ECQUSF14CT	1 mL	50/Pack	150 mg MgSO <sub>4</sub> 50 mg PSA
ECQUSF24CT	1 mL	50/Pack	150 mg MgSO₄ 50 mg PSA 50 mg C18
ECQUSF34CT	1 mL	50/Pack	150 mg MgSO <sub>4</sub> 25 mg PSA 2.5 mg GCB
ECQUSF44CT	1 mL	50/Pack	150 mg MgSO <sub>4</sub> 50 mg PSA 50 mg C18 7.5 mg GCB
ECQUSF54CT	1 mL	50/Pack	150 mg MgSO <sub>4</sub> 50 mg PSA 50 mg C18 50 mg Chloro- filtr <sup>®</sup>
ECQUSF64CT	1 mL	50/Pack	150 mg MgSO₄ 50 mg C18 50 mg Chloro- filtr®
ECQUSF74CT	1 mL	50/Pack	150 mg MgSO <sub>4</sub> 50 mg C18

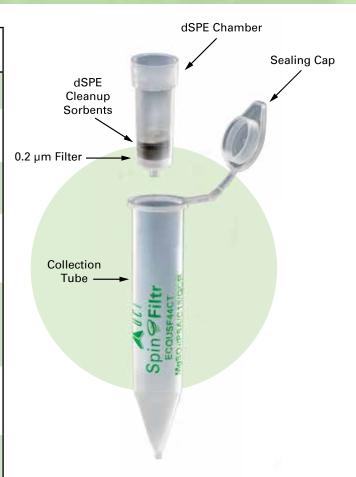

# Discover a whole new approach to dSPE!



The easy-to-use Lipifiltr® push-thru cartridge was designed to remove lipids from acetonitrile extracts. Samples are extracted using a standard QuEChERS procedure and an aliquot of the supernatant is simply pushed through the Lipifiltr® purification cartridge using a disposable syringe. The purified extract is collected in an autosampler vial and analyzed by UHPLC-MS/MS. The ability to obtain significantly cleaner extracts, ease of use, and time and cost savings make the new Lipifiltr® push-thru cartridges an attractive cleanup option for laboratories conducting pesticide residue analysis in complex fatty samples.

LipiFiltr® Push Thru Cartridge		
Part Number	Unit	
LPFLTR01	50/Pack	




### **Gravimetric Analysis:**

The performance of the LipiFiltr<sup>®</sup> push-thru cartridges to remove lipids and other matrix components was evaluated gravimetrically by collecting 2 mL of sample before and after cleanup in pre-weighed test tubes and heating them to dryness at 110° C in an oven.

Matrix	Matrix Removal (%)
Beef	79.1
Black Olives	84.3
Avocado	54.7
Salmon	80.9
Chicken fat	71.7
Olive oil	61.5
Nuts	84.3
Swordfish	80.9

# **Extract Concentration Before and After LipiFiltr® Cleanup:**

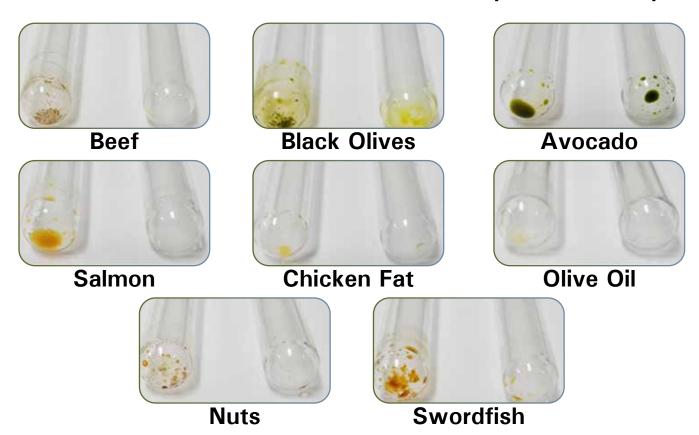

# **QuICK QuEChERS**

Simple, Fast, Efficient Cartridges for Clean-Up of QuEChERS Extracts


UCT's QuICK QuEChERS push-thru cartridge eliminates the need for shaking and centrifugation of extracts during clean-up, significantly reducing sample processing time. In addition, any residual sorbent is filtered via the frit providing a clean, final extract for analysis.\*

#### After QuEChERS sample extraction:

- 1. Draw the extract into a disposable syringe
- 2. Push the extract through the cartridge into a sample vial
- 3. Sample is ready for analysis by LC or GC

The UCT QuICK QuEChERS Cartridge provides results comparable to traditional dSPE but without the need for centrifugation.



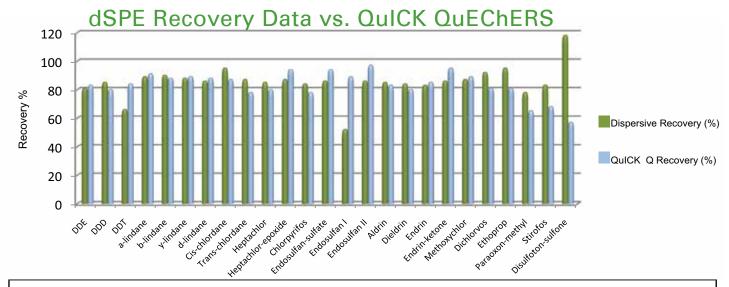

Part Number	Cartridge Size	Contents
ECPURMPSMC	Medium	110 mg MgSO <sub>4</sub> (top layer); PTFE Frit; 180 mg PSA (bottom layer)
ECPURMPSLC	Large	110 mg MgSO <sub>4</sub> (top layer); PTFE Frit; 600 mg PSA (bottom layer)

<sup>\*</sup> Product developed by Steven C. Moser - OK Department of Agriculture, Food and Forestry

# **SPE Dual Phase Cartridge Clean-up**



SPE dual phase cartridges provide an alternative clean-up option for complicated matrices and/or when dSPE does not provide adequate cleanliness of sample extracts. Examples of matrices that are suitable for SPE include tea, herbs, spices and high lipid content samples.

Part Number	Volume	Quantity	Frit Type	Contents
ECPSACB6	6 mL	30/Pack	PTFE	200 mg GCB 400 mg PSA
ECPSACB256	6 mL	30/Pack	PTFE	250 mg GCB 500 mg PSA
ECPSACB256-PE	6 mL	30/Pack	PE	250 mg GCB 500 mg PSA
ECPSACB21M6	6 mL	30/Pack	PTFE	250 mg GCB 1000 mg PSA
ECPSACB506	6 mL	30/Pack	PTFE	500 mg GCB 500 mg PSA
ECPSACB506P	6 mL	30/Pack	PE	500 mg GCB 500 mg PSA
ECNAXCB506	6 mL	30/Pack	PTFE	500 mg GCB 500 mg CUNAX
EUMSPSA6	6 mL	30/Pack	PTFE	500 mg PSA 750 mg MgSO <sub>4</sub>
ECPSAC1856	6 mL	30/Pack	PTFE	500 mg PSA 500 mg C18
ECMSPSACB6	6 mL	30/Pack	PTFE	250 mg GCB 500 mg PSA 750 mg MgSO <sub>4</sub>
EUSILMSSM26	6 mL	30/Pack	PTFE	1000 mg silica 200 mg muffled anhydrous sodium sulfate
EUCARBC18515	15 mL	20/Pack	PTFE	500 mg GCB 500 mg C18
EEMSC1811M15	15 mL	20/Pack	PTFE	1000 mg C18 1000 mg MgSO <sub>4</sub>
EEMS2C181M15	15 mL	20/Pack	PFTE	1000 mg C18 2000 mg MgSO <sub>4</sub>
EUPSAC181M15	15 mL	20/Pack	PTFE	1000 mg PSA 1000 mg C18

# Enviro-Clean Universal & Specialty Cartridges




# **Universal Cartridges**



UNIVERSAL
OIL & GREASE



UNIVERSAL 525



UNIVERSAL PAH / DRO



UNIVERSAL C18



UNIVERSAL 549




UNIVERSAL Zero-Blank Filter™

Part Number	Product Name	Description	Quantity	Amount/Tube Vol.
ECUNIOGXF	UNIVERSAL OIL & GREASE	For EPA Method 1664/ Sorbent C18	15/Pack	2000 mg / 83 mL
ECUNI525	UNIVERSAL 525	For EPA Method 525.2 & 525.3 / Sorbent C18	8/Pack	1500 mg / 83 mL
ECUNIPAH	UNIVERSAL PAH / DRO	For PAH and Diesel Range Organics extractions/ Sorbent C18	8/Pack	2000 mg / 83 mL
ECUNIC18	UNIVERSAL C18	For extraction of pesticides, herbicides and PCBs, etc./ Sorbent C18	8/Pack	1100 mg / 83 mL
ECUNI549	UNIVERSAL 549	For EPA Method 549/ Sorbent C8	8/Pack	500 mg / 83 mL
ECUNIDVB500	UNIVERSAL DVB	For extraction of a wide range of analytes/ Sorbent PS-DVB	8/Pack	500 mg / 83 mL
ECBLANK	UNIVERSAL Zero-Blank Filter™	Proprietary adsorbent for filtration of lab air for use during sorbent drying	6/Pack	200 mg / 83 ml

#### **ENVIRO-CLEAN®**

#### **UNIVERSAL CARTRIDGE RESERVOIRS**

Part Number	Description	Quantity
ERFT1FUNIP	1 10µm PTFE frit	10/Pack
ERFT2FUNIP	2 10µm PTFE frits	10/Pack
ERTFT1FUNIP	1 50µm PTFE frit	10/Pack
ERFV00UNIP	Empty Reservoir	10/Pack

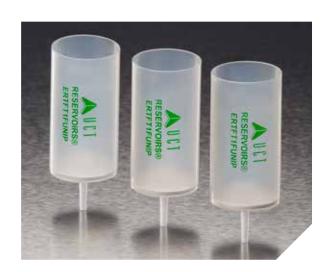


FITS THE HORIZON SPE-DEX® 4790 AUTOMATED EXTRACTION SYSTEM

### For Environmental & EPA Extractions

Product Name	Description	Part Number	Amount/Tube Vol.	Units/Pack
Clean-Elute™	Diatomaceous Earth for EPA Method 509	CLEAN-ELUTE	25,000 mg / 200mL	108
Enviro-Clean <sup>®</sup> HL DVB	For use in EPA Methods 526, 528, 529, 530, 544, 553, 1694, 8321B, 8141B, 8330	ECHLD156-P	500 mg / 6mL	30
Enviro-Clean® 521 & 522	Activated Carbon for EPA Methods 521 & 522	EU52112M6	2000 mg / 6mL	30
Enviro-Clean® 523	Graphitized Carbon for EPA Method 523	EC5232506	250 mg / 6mL	30
Enviro-Clean® 525	Novel C18 blend for use in EPA Method 525.2	EC525006	1500 mg / 6mL	30
Enviro-Clean® 535 (90 m²/g SA)	For EPA Method 535 or in applications requiring Graphitized Carbon Black with lower surface area	EC535156	500 mg / 6mL	30
Enviro-Clean® 537	For EPA Method 537 Perfluorinated Alkyl Acids	ECHLD156-P	500 mg / 6mL	30
Enviro-Clean <sup>®</sup> 541	For EPA Method 541 Polar Organic Compounds in Drinking Water	EU541163	600 mg / 3mL	50
Enviro-Clean® 548	For EPA Method 548.1 Endothall Extraction	EC548006	548 Slurry / 6mL	30
Enviro-Clean <sup>®</sup> C8	For EPA Method 549 Diquat & Paraquat	EEC08156	500 mg / 6mL	50
Enviro-Clean® EPH Fractionation	Developed for fractionation of MA EPH (gravity flow)	XRSIHT13M15 XRSIHT15M25 CUSILHT15M25	3000 mg / 15mL 5000 mg / 25mL 5000 mg / 25mL	24 20 20
Enviro-Clean® Silica Gel	For silica gel clean-up applications	EUSILMSSM26	1000 mg silica: 200 mg muffled anhydrous sodium sulfate / 6mL	30
Enviro-Clean® Anhydrous Sodium Sulfate Drying Cartridge	Used for the removal of water from extracts prior to concentration and analysis	ECSS15M6	5000 mg / 6mL	30
Enviro-Clean® Anhydrous Sodium Sulfate Muffled – Glass Reservoir	Used for the removal of water from extracts prior to concentration and analysis	CUSS25M6G	2500 mg / 6mL	30
Enviro-Clean® Alumina & Silica Dual-Phase Cartridge	For environmental clean-up	ECALNSIL25M25	2500 mg alumina neutral: 5000 mg silica / 25mL	20
Enviro-Clean® Sodium Sulfate & Florisil Dual-Phase Cartridge	For environmental clean-up	EUSSFL2M6	2000 mg sodium sulfate: 2000 mg florisil / 6mL	30

#### **ENVIRO-CLEAN® HL DVB**

ENVIRO-CLEAN® HL DVB extraction columns are manufactured from an extremely clean, highly cross-linked divinylbenzene based sorbent. The material was developed with the environmental market in mind. It has been successfully used to extract a wide range of analytes from water samples. By varying the sample pH, wash and elution solvents ENVIRO-CLEAN® HL DVB can be used to analyze acidic, basic, and neutral (both polar & non-polar) compounds.

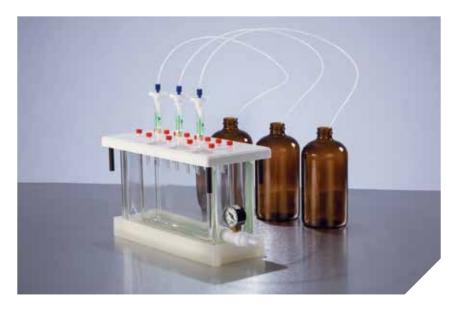

Part Number	Description	Quantity
ECHLD(150)6-P	150 mg / 6mL Cartridge	30/Pack
ECHLD126-P	200 mg / 6mL Cartridge	30/Pack
ECHLD156-P	500 mg / 6mL Cartridge	30/Pack



www.unitedchem.com

# EPA METHOD 8270 - Extraction of Acids, Bases, and Neutrals in Water using Solid Phase Extraction

UCT offers a 2 cartridge system and extraction procedure for EPA Method 8270. A wide range of 137 target analytes and 6 surrogates can be successfully analyzed using this method. The procedure is reliable, efficient, and cost-effective. The tandem cartridge system uses UCT's proprietary 8270 cartridge in-line with our activated carbon cartridge. High throughout can be achieved by extracting multiple samples simultaneously using a multi-port SPE manifold combined with a 12 position collection rack, which allows for the simultaneous extraction of up to 12 samples at once. A set of 24 samples can be extracted in 5 to 6 hours.

#### **Product Benefits**

- Cost-effective
- Reduced usage of organic solvents
- Only one sample pass is needed
  - 5-6 hrs for a batch of 24 samples.
- No emulsion or white precipitate generated
- Shorter solvent evaporation time
- Shorter sample turnaround time
- High sample throughput
- Excellent recovery
- Cleaner extracts and chromatograms
- Cartridge body manufactured from special, proprietary polypropylene – minimizing potential source of interferences
- Packaged in Mylar to maintain cleanliness





### 8270 Cartridge Kits

	1 Liter Sample Size	
Part Number	Description	Quantity
EC8270-KIT1L	ENVIRO-CLEAN® 8270 STARTER KIT	Kit
Contents	30 x 8270 Extraction Cartridges (p/n EC82702M15), 30 x Carbon Extraction Cartridges (p/n EU52113M6), 30 x Cartridge Adapters (p/n AD0000AS), 12 x Large Volume Transfer Tubes (p/n VMFSTFR12)	
EC8270-1000REFL	ENVIRO-CLEAN® 8270 REFILL KIT	Kit
Contents	30 x 8270 Extraction Cartridges (p/n EC82702M15), 30 x Carbon Extraction Cartridges (p/n EU52113M6)	
	500 mL Sample Size	
Part Number	Description	Quantity
EC8270-KIT	ENVIRO-CLEAN® 8270 STARTER KIT	Kit
Contents	30 x 8270 Extraction Cartridges (p/n EC82701M15), 30 x Carbon Extraction Cartridges (p/n EU52112M6), 30 x Cartridge Adapters (p/n AD0000AS), 12 x Large Volume Transfer Tubes (p/n VMFSTFR12)	
EC8270-500REFL	ENVIRO-CLEAN® 8270 REFILL KIT	Kit
Contents	30 x 8270 Extraction Cartridges (p/n EC82701M15), 30 x Carbon Extraction Cartridges (p/n EU52112M6)	
	< 100 mL Sample Size	
Part Number	Description	Quantity
EC8270-KIT100ML	ENVIRO-CLEAN® 8270 STARTER KIT	Kit
Contents	30 x 8270 Extraction Cartridges (p/n EC8270506), 30 x Carbon Extraction Cartridges (p/n EU5211M6), 30 x Cartridge Adapters (p/n AD0000AS), 12 x Large Volume Transfer Tubes (p/n VMFSTFR12)	
EC8270-100REFL	ENVIRO-CLEAN® 8270 REFILL KIT	Kit
Contents	30 x 8270 Extraction Cartridges (p/n EC8270506) 30 x Carbon Extraction Cartridges (p/n EU5211M6)	

	8270 Cartridge Refills				
Part Number	Quantity				
EC8270506	500 mg in a 6mL Cartridge	30/Pack			
EC82701M15	1000 mg in a 15mL Cartridge	30/Pack			
EC82702M15	2000 mg in a 15mL Cartridge	30/Pack			

	Carbon Cartridge Refills				
Part Number	Description	Quantity			
EU5211M6	1000 mg in a 6mL Cartridge	30/Pack			
EU52112M6	2000 mg in a 6mL Cartridge	30/Pack			
EU52113M6	3000 mg in a 6mL Cartridge	30/Pack			

# **Extraction Manifold**

Part Number	Description	Quantity
VMF016GL	16 Position Complete Vacuum Manifold System	Complete Unit
Contents	1 x Glass Block 1 x 16 Position Corian Lid 1 x Cover Gasket 1 x Vacuum Gauge 1 x 16 Position Adjustable Collection Rack 1 x Glass Block Safety Tray 16 x PTFE Tips 16 x Bulkhead Luer Fittings 16 x Plugs	

#### **ENVIRO-CLEAN® Push-Thru Purification Cartridges**

UCT's wide sorbent range is also offered in a convenient push-thru format, providing simple, fast, and efficient sample clean-up. The analyst can choose from a wide range of sorbent types tailored to the specific requirements of each analysis. The small, medium, and large push-thru cartridges allow for the filtration and removal of unwanted matrix that can otherwise lead to significant ion suppression during sample analysis.







**SMALL** 


**MEDIUM** 

**LARGE** 

Part Number	Cartridge Size	Quantity	Frit Type	Contents
EEC1815MC	Medium	50/Pack	PTFE	Enviro-Clean® Encapped C18
EEC18MC-P	Medium	50/Pack	PE	Enviro-Clean® Encapped C18
EUCARBMC	Medium	30/Pack	PTFE	Enviro-Clean® Graphitized Carbon – 120/400 Mesh
EUFLSLC	Large	50/Pack	PTFE	Enviro-Clean® Florisil® PR
EUALNLC-P	Large	50/Pack	PE	Enviro-Clean® Alumina Neutral
EUQAXLC	Large	50/Pack	PTFE	Enviro-Clean® Quaternary Amine
EUPSAMC	Medium	50/Pack	PTFE	Enviro-Clean® Primary/ Secondary Amine
EUPSALC	Large	50/Pack	PTFE	Enviro-Clean® Primary/ Secondary Amine

#### **ENVIRO-CLEAN® Push-Thru Glyphosate Purification Cartridges**

Remove unwanted matrix interferences that can lead to significant suppression and loss of ionization for glyphosate and glufosinate. Water and vegetation/fruits/swabs and other non-soil samples extracted with water are simply pushed through the Glyphosate cartridge to purify final extracts.

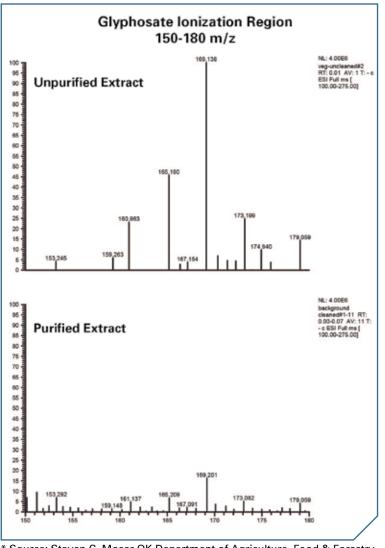



Part Number	Size	Contents	
ECGLYSC	Small Cartridge	180 mg*	
ECGLYLC	Large Cartridge	560 mg*	
* Proprietary polymeric sorbent blend			

<sup>\*</sup> Source: Steven C. Moser OK Department of Agriculture, Food & Forestry


\*\*Glyphosate is found at 168 m/z in ESI mode.

Infused samples were injected onto LC/MS Ion Trap in full scan mode for an average of a 30 second infusion pre and post clean-up using UCT's Glyphosate Purification Cartridges. Background matrix peaks that can lead to significant suppression and compete with glyphosate and glufosinate during ionization were significantly reduced following clean-up.

# ENVIRO-CLEAN® Fusion®Ag+


Fractionation of aliphatic and aromatic hydrocarbons are routinely assessed to identify the risks posed by petroleum in the environment. Solid Phase Extraction (SPE) with heat-treated silica gel is the traditional approach for the fractionation of aliphatic and aromatic hydrocarbons.

The biggest challenge of this approach is the deactivation of the silica gel due to its hygroscopic nature, which leads to inconsistent results, incomplete separation, and low recoveries. The process to optimize each batch of silica cartridges is time consuming and exhausts copious amounts of hexane solvent.

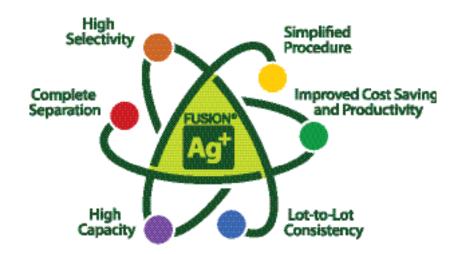

UCT's Enviro-Clean Fusion® Ag+ SPE sorbent is designed to help overcome


the challenges associated with traditional silica gel fractionation. The new EPH fractionation sorbent consists of silver ions anchored onto a solid support to provide the best selectivity, capacity, and performance.

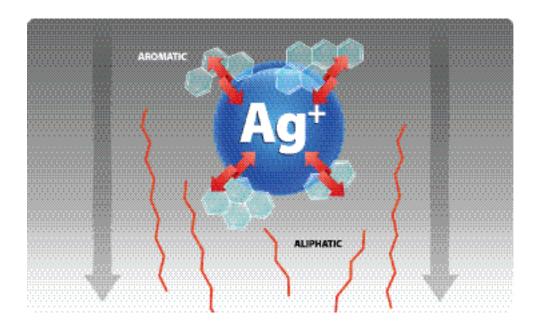


Aromatic hydrocarbons form a charge-transfer complex with silver ions ensuring complete separation of aliphatic from aromatic fractions without breakthrough.

Figure 2 - Illustration of Ag<sup>+</sup> interaction with aromatic and aliphatic hydrocarbons

ENVIRO-CLEAN® Fusion® Ag <sup>+</sup> Order Information					
Description Part Number					
Fusion® Ag <sup>+</sup> / 0.5 g, 6mL cartridge	ECFUSAG156				
Fusion® Ag <sup>+</sup> / 1 g, 6mL cartridge	ECFUSAG1M6				
Fusion® Ag <sup>+</sup> / 2 g, 6mL cartridge	ECFUSAG2M6				

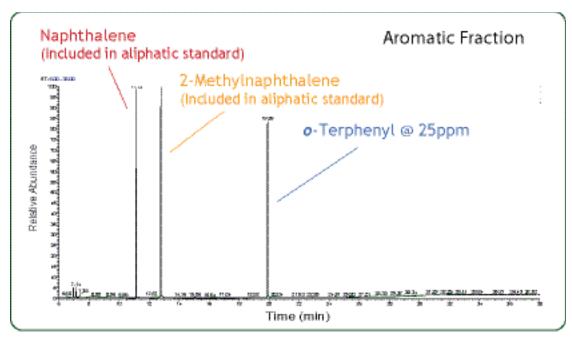

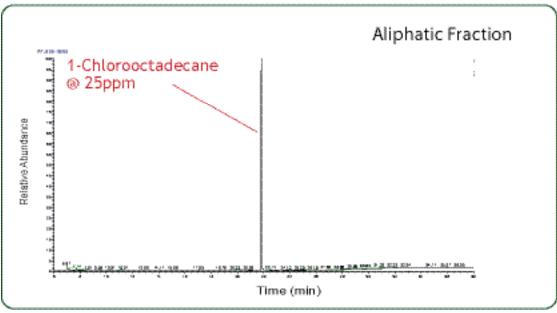

**Experiment conditions**: Fusion<sup>®</sup> Ag+ 1g/6mL cartridge; Sample: NJDEP EPH 10/08 Rev.2 aliphatics calibration standard and aromatic calibration standard; Concentration: 200  $\mu$ g/mL in hexane; GC-MS system: Thermo Trace 1300 GC & ISQ MS; Restek Rxi<sup>®</sup>-5sil MS, 30m x 0.25mm, 0.25 $\mu$ m with Integra-Guard; Injection volume: 1 $\mu$ L split (1:100) at 300°C; GC liner: 4 mm split liner with deactivated glass wool; Temperature: Transfer line = 275°C; lon source = 275°C; Oven temp. program: Initial temperature at 50°C, hold for 3 min; ramp at 10°C/min to 320°C, hold for 10 min; Full scan range: 35-600 amu.

# ENVIRO-CLEAN® Fusion®Ag+

Fusion® Ag+ requires less solvent consumption and reduced extraction times as compared to silica cartridges with a similar configuration (Table 2, 3). Due to the strong ionic interaction of the silver ions with the aromatic hydrocarbon fraction, there is no need to optimize the hexane volume for each lot of silica cartridges. This results in a simplified process procedure.

Fewer solvent requirements and shortened extraction time improves cost efficiencies and laboratory productivity. The small configurations: 0.5g/6mL and 1g/6mL are ideal for automated high throughput analysis. The 2g/6mL configuration is best for higher loading capacity. In addition, using acetone instead of dichloromethane as the elution solvent for the aromatic fraction is more environmentally friendly.


Table 2 - Fusion® Ag+ reduces solvent consumption


		Solvent Cor	nsumption (mL)
Extraction Steps		Fusion® Ag* 1g/6mL	Heat-treated Silica 2g / 6mL
Conditioning	Acetone	4	
	Dichloromethane		3
	Hexane	4	6
Sample Loading	Sample Loading Hexane		1
Aliphaticfraction	Hexane	4	4
Aromatic fraction	Acetone	4	
	Dichloromethane		6
Total solvent consumption (ml)		9	20
Total chlorinated	solvent used (mL)	0	9

Table 3 - Fusion® Ag+ shortens extraction time




		Extraction	Time (min)
Extract	ion Steps	Fusion® Ag+ H 1g/6mL	eat-treated Silica 2g/6mL
Conditioning	Acetone	1.8	
	Dichloromethane (5-minhold)		5.8
Sample Loading	Hexane	1.7	1.9
Aliphatic fraction Hexane		0.5	0.5
Aromaticfraction	Hexane	1.7	1.4
	Acetone	1.5	
	Dichloromethane		2.8
Total extraction time (min)		7.2	12.4

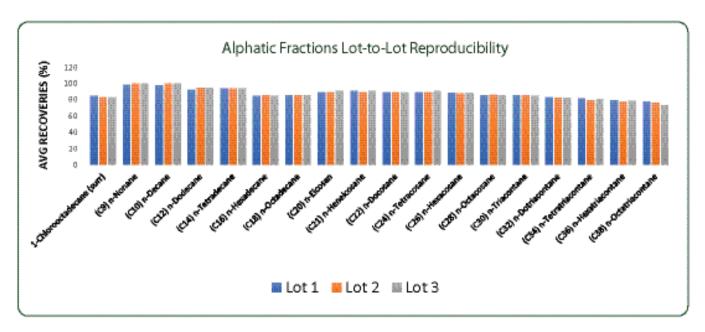

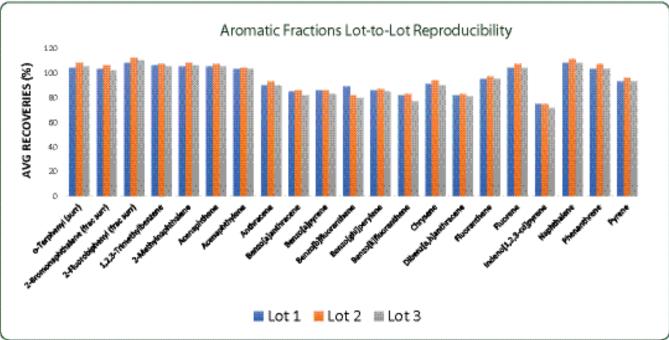

Experimental conditions are the same as Figure 3. Three samples were tested from each lot.

# ENVIRO-CLEAN® SOLID-PHASE EXTRACTION CARTRIDGES

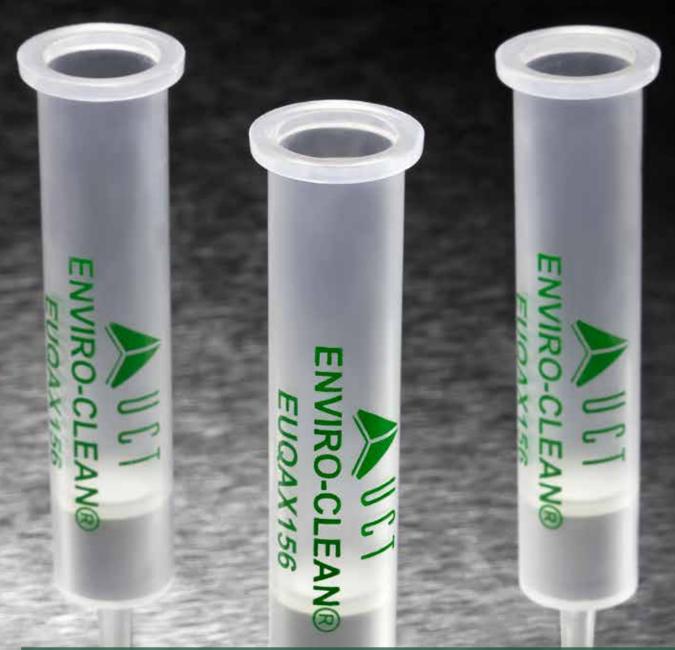

HYDROPHOBIC / HYDROPHILIC / ION EXCHANGE / COPOLYMERIC / POLYMERIC

#### **ENVIRO-CLEAN® SORBENTS**

ENVIRO-CLEAN® solid-phase extraction (SPE) cartridges are designed specifically for the isolation and purification of environmental analytes such as pesticides, herbicides, polyaromatic hydrocarbons, polychlorinated biphenyls and other environmentally related compounds. By utilizing ultra-clean extraction sorbents along with chemically resistant PTFE frits, an end-user not only has the ability to purify complex matrices, but also reduce ion suppression or enhancement, and most importantly enrich compunds present at trace concentration levels.

To successfully conduct SPE, a mechanistic understanding of the interaction between sorbent and analyte of interest is vital for producing optimal results. The most common retention mechanisms include non-polar interactions (van der Waals forces), polar interactions (hydrogen bonding, dipoledipole forces), and ionic interactions (cation-anion exchange).

Non-polar phases are universal but often are considered to exhibit the least selective retention mechanisms when compared to normal phase or ion-exchange SPE. C18 is the most widely used of these phases. While this retention mechanism happens to lack specificity, it is very useful for extracting analytes that are very diverse in structure within the same sample. Several EPA approved methods for analyzing organics in water mandate the use of a C18 phase.

Retention of an analyte under normal phase conditions is primarily due to interactions between polar functional groups of the analyte and polar groups on the sorbent surface. This could include hydrogen bonding, pi-pi, and dipole-dipole interactions. This mode is classically used to separate neutral organic compounds whose chemical nature ranges from hydrophobic to moderately polar.

lon-exchange phases are often applied when analytes of interest carry a charge while in solution. The primary retention mechanism of the compound is based mainly on the electrostatic attraction of the charged functional group on the compound to the charged group that is bonded to the sorbent surface. ENVIRO-CLEAN® sorbents are available in either cation or anion exchangers and exhibit both weak and strong characteristics.

Lastly, copolymeric phases offer a dual retention mechanism providing superior cleanliness. Hydrophobic interactions in addition to ion exchange contribute to a higher degree of analyte selectivity than what was previously possible. Compounds of interest can be retained by multiple mechanisms, resulting in greater removal of matrix-related contamination.


#### **SPE TERMINOLOGY**

- Sorbent -The solid-phase material to which analytes attach during the extraction process
- Bed Volume The quantity of solvent needed to cover the sorbent
- Capacity The amount of analyte that a sorbent can retain
- Activation a process of rinsing the sorbent with a solvent to clean the bed and extend the bonded groups (i.e. C18) to maximize its effectiveness
- Wash Solvent Solvent used to wash interferences off of the sorbent prior to elution
- Retention The attraction a solid-phase has for the analyte that causes the analyte to "adsorb" to the sorbent
- Elution The process of removing an analyte from the sorbent for analysis

### **ENVIRO-CLEAN® SOLID PHASE EXTRACTION CARTRIDGES**

#### **HOW TO READ ENVIRO-CLEAN® PART NUMBERS:**

#### **ENVIRO-CLEAN® CODE**

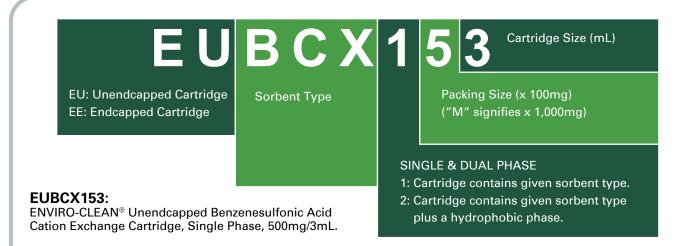

#### **Sorbent Type**


CODE	DESCRIPTION
C08, C18, C30	Carbon Chains
SIL	Unbonded Silica
PSA	n-2 Aminoethyl
BCX	Benzenesulfonic Acid Cation Exchanger
PCX	Propylsulfonic Acid Cation Exchanger
CCX	Carboxylic Acid Cation Exchanger
QAX	Quaternary Amine Anion Exchanger
NAX	Aminopropyl Anion Exchanger
FLS	Florisil® PR
ALA	Alumina - Acid
ALB	Alumina - Base
ALN	Alumina - Neutral
CNP	Cyanopropyl
CYH	Cyclohexyl
DOL	Diol
PHY	Phenyl

#### HYDROPHOBIC EXTRACTION SORBENTS

UCT's ENVIRO-CLEAN® hydrophobic sorbents feature silanol groups at the surface of the raw silica packing that have been chemically modified with hydrophobic alkyl or aryl functional groups. These phases are commonly utilized to extract compounds that exhibit medium non-polar characteristics from a variety of complex matrices. The C18 phase is the most widely used phase for non-polar interactions because of its non-selective nature; C18 will extract a large number of compounds with differing chemical properties. To enhance selectivity, UCT offers a variety of hydrophobic sorbents ranging from C2 all the way to C30, as well as endcapped and unendcapped versions.

#### MECHANISM OF HYDROPHOBIC BONDING


Retention of organic analytes from polar solutions (e.g. water) onto these SPE materials is due primarily to the attractive forces between the carbon-hydrogen bonds in the analyte and the functional groups. These nonpolar-nonpolar attractive forces are commonly called van der Waals forces, or dispersion forces. To elute an adsorbed compound from a reversed phase sorbent, use a nonpolar solvent to disrupt the forces that bind the compound to the packing. Some polar solvents, such as methanol and acetonitrile have enough non-polar characteristics to disrupt nonpolar binding triggering compound elution. Methanol can be used as well, although it should be noted that it will remove both polar and non-polar analytes of interest as well as interferences.

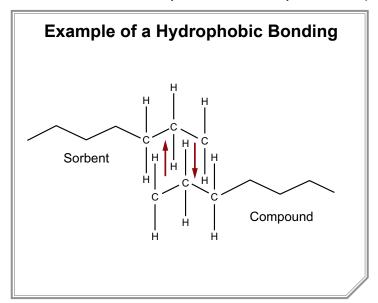

Hydrophobic Sorbents & Structures			
Sorbent	Structure		
C2 Ethyl	-SiCH <sub>2</sub> CH <sub>3</sub>		
C4 n-Butyl	-Si(CH <sub>2</sub> ) <sub>3</sub> CH <sub>3</sub>		
C8 Octyl	-Si(CH <sub>2</sub> ) <sub>7</sub> CH <sub>3</sub>		
C18 Octadecyl	-Si(CH <sub>2</sub> ) <sub>17</sub> CH <sub>3</sub>		
C30 Tricontyl	-Si(CH <sub>2</sub> ) <sub>29</sub> CH <sub>3</sub>		
Cyclohexyl	-Si —		
Phenyl	-Si —		

#### ENDCAPPED VS. UNENDCAPPED

Bonded phases are manufactured by the reaction of organosilanes with activated silica. During the polymerization reaction of carbon chains to the silica backbone, a very stable silyl ether linkage forms. Our unendcapped columns allow hydroxyl sites to remain, thus making these columns slightly hydrophilic. In order to minimize this slight polarity, the hydroxyl sites are deactivated. Proprietary bonding techniques ensure that these sites are 100% reacted, leading to complete endcapping. Because there are no hydroxyl sites left, our endcapped columns render the silica non-acidic and non-polar.

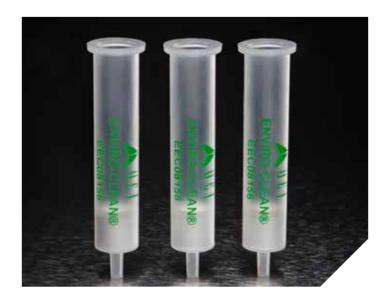

C18, OCTADECYL

Organic Loading = 21.5%Surface Area =  $500 \text{ m}^2/\text{g}$ 

Average Pore Size = 60ÅPore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

Orga

C8, OCTYL Organic Loading = 11.1% Surface Area = 500 m<sup>2</sup>/g

Average Pore Size =  $60\text{\AA}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

	COLUMNS					
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Endcapped	Part Number		
1	50	100	NO	EUC181L1		
1	100	100	NO	EUC18111		
1	100	100	YES	EEC18111		
3	200	50	NO	EUC18123		
3	200	50	YES	EEC18123		
3	500	50	NO	EUC18153		
3	500	50	YES	EEC18153		
6	500	50	NO	EUC18156		
6	500	50	YES	EEC18156		
6	1000	30	NO	EUC181M6		
6	1000	30	YES	EEC181M6		
10	100	50	NO	EUC1811Z		
10	100	50	YES	EEC1811Z		
10	200	50	NO	EUC1812Z		
10	200	50	YES	EEC1812Z		
10	500	50	NO	EUC1815Z		
10	500	50	YES	EEC1815Z		
15	1000	20	YES	EEC1811M15		
15	2000	20	NO	EUC1812M15		
15	2000	20	YES	EEC1812M15		
25	5000	20	NO	EUC1815M25		
25	5000	20	YES	EEC1815M25		
75	10000	10	NO	EUC18110M75		
75	10000	10	YES	EEC18110M75		

COLUMNS					
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Endcapped	Part Number	
1	50	100	NO	EUC081L1	
1	100	100	NO	EUC08111	
1	100	100	YES	EEC08111	
3	200	50	NO	EUC08123	
3	200	50	YES	EEC08123	
3	500	50	NO	EUC08153	
3	500	50	YES	EEC08153	
6	500	50	NO	EUC08156	
6	500	50	YES	EEC08156	
6	1000	30	NO	EUC081M6	
6	1000	30	YES	EEC081M6	
10	100	50	NO	EUC0811Z	
10	200	50	NO	EUC0812Z	
10	200	50	YES	EEC0812Z	
10	500	50	NO	EUC0815Z	
10	500	50	YES	EEC0815Z	
15	2000	20	NO	EUC0812M15	
15	2000	20	YES	EEC0812M15	
25	5000	20	NO	EUC0815M25	
25	5000	20	YES	EEC0815M25	
75	10000	10	NO	EUC08110M75	
75	10000	10	YES	EEC08110M75	

# **ENVIRO-CLEAN®**

### Hydrophobic Phase

#### C2, ETHYL

Organic Loading = 6.2%Surface Area =  $500 \text{ m}^2/\text{g}$  Average Pore Size =  $60\text{\AA}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

	COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Endcapped	Part Number	
6	500	50	YES	EEC02156	
10	500	50	YES	EEC0215Z	

#### C30, TRICONTYL

Organic Loading = 20.0% Surface Area = 500 m<sup>2</sup>/g Average Pore Size = 60ÅPore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

	COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Endcapped	Part Number	
3	200	50	NO	EUC30123	
3	500	50	NO	EUC30153	
6	1000	30	YES	EEC301M6	
10	500	50	NO	EUC3015Z	
10	500	50	YES	EEC3015Z	

#### PHY, PHENYL

Organic Loading = 10.8%Surface Area =  $500 \text{ m}^2/\text{g}$  Average Pore Size = 60ÅPore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Endcapped	Part Number
3	500	50	NO	EUPHY153
3	500	50	YES	EEPHY153
6	1000	30	NO	EUPHY1M6

#### CYH, CYCLOHEXYL

Organic Loading = 11.6%Surface Area =  $500 \text{ m}^2/\text{g}$  Average Pore Size = 60ÅPore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

COLUMNS					
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Endcapped	Part Number	
3	500	50	NO	EUCYH153	
6	500	50	YES	EECYH156	
6	1000	30	YES	EECYH1M6	




#### **ENVIRO-CLEAN® HYDROPHILIC NORMAL PHASE EXTRACTION SORBENTS**

Hydrophilic sorbents are composed of a silica backbone bonded with carbon chains containing polar functional groups. Examples of phases that feature this functionality include bare silica, diol, and cyanopropyl phases.

### Mechanism of Hydrophilic Bonding

Compounds are retained on hydrophilic sorbents through polar interactions including hydrogen bonding, pi-pi or dipole-dipole interactions. These types of interactions occur when the distribution of electrons between individual atoms in functional groups is unequal, causing negative and positive polarity. Polar-functionalized bonded silicas and polar adsorption media are typically used under normal phase conditions.

Hydrophilic Sorbents & Structures		
Sorbent	Structure	
Silica	-SiOH	
Diol	-Si(CH <sub>2</sub> ) <sub>3</sub> OCH <sub>3</sub> OHCH <sub>2</sub> OH	
Cyanopropyl	-Si(CH <sub>2</sub> ) <sub>3</sub> CN	

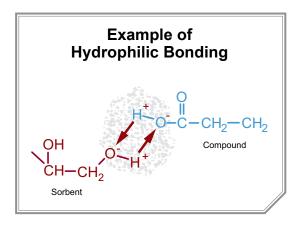

## **ENVIRO-CLEAN®**

## **Hydrophilic Phase**

#### UNBONDED SILICA, ACID WASHED

Organic Loading = N/A Surface Area = 500 m<sup>2</sup>/g Average Pore Size = 60ÅPore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

#### PHARMA-SIL®

Organic Loading = N/ASurface Area =  $500 \text{ m}^2/g$  Average Pore Size = 60ÅPore Volume =  $0.82 \text{ cm}^3/\text{g}$ 

	COLUMNS				
Tube Volume (mL)	Volume Amount		Part Number		
1	100	100	EUSIL111		
3	200	50	EUSIL123		
3	500	50	EUSIL153		
6	500	50	EUSIL156		
6	1000	30	EUSIL1M6		
15	2000	20	EUSIL12M15		
25	5000	20	EUSIL15M25		
75	10000	10	EUSIL110M75		

	COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number		
1	100	100	EPHSIL111		
3	500	50	EPHSIL153		
6	500	50	EPHSIL156		
6	1000	30	EPHSIL1M6		
10	200	50	EPHSIL12Z		
15	2000	20	EPHSIL12M15		
25	5000	20	EPHSIL15M25		
75	10000	10	EPHSIL110M75		

#### **ALUMINA, ACIDIC**

	COLUMNS				
Tube Volume (mL)	Volume Amount		Part Number		
3	200	50	EUALA123		
3	500	50	EUALA153		
6	500	50	EUALA156		
6	1000	30	EUALA1M6		
6	2000	30	EUALA2M6		
15	2000	20	EUALA12M15		

#### **ALUMINA, BASIC**

	COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number		
1	50	100	EUALB1L1		
3	500	50	EUALB153		
6	500	50	EUALB156		
6	1000	30	EUALB1M6		
15	2000	20	EUALB12M15		

#### **ALUMINA, NEUTRAL**

	COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg) Units per Pack		Part Number		
1	50	100	EUALN1L1		
1	100	100	EUALN111		
3	200	50	EUALN123		
6	500	50	EUALN156		
6	1000	30	EUALN1M6		
15	2000	20	EUALN12M15		
25	5000	20	EUALN15M25		
75	10000	10	EUALN110M75		


#### DIOL

Organic Loading = 8.0%Surface Area =  $500 \text{ m}^2/\text{g}$  Average Pore Size = 60 ÅPore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number	
1	50	100	EUDOL1L1	
1	100	100	EUDOL111	
1	200	100	EUDOL121	
3	200	50	EUDOL123	
3	500	50	EUDOL153	
6	500	50	EUDOL156	
6	1000	30	EUDOL1M6	
10	500	50	EUDOL15Z	
15	2000	20	EUDOL12M15	
25	5000	20	EUDOL15M25	

#### CARBON, GRAPHITIZED NON-POROUS, 120/400 MESH

COLUMNS				
Tube Volume (mL)	Sorbent Units per Amount (mg) Pack		Part Number	
1	100	100	EUCARB111	
3	200	50	EUCARB123	
3	500	50	EUCARB153	
6	200	50	EUCARB126	
6	250	30	EUCARB2L6	
6	500	50	EUCARB156	
6	1000	30	EUCARB1M6	
10	100	50 EUCARE		
10	200	50	EUCARB12Z	
15	2000	20	EUCARB12M15	

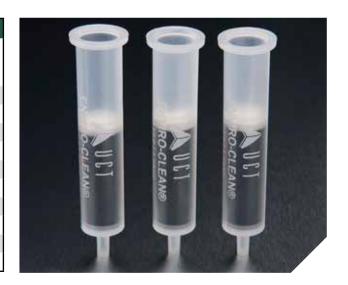

FLORISIL® PR Florisil® is the trademark of U.S. Silica Co.

	COLUMNS				
Tube Volume (mL)	Sorbent Units p Amount (mg) Pack		Part Number		
1	100	100	EUFLS111		
3	200	200 50 <b>E</b>			
3	500	50	EUFLS153		
6	500	50	EUFLS156		
10	100	50	EUFLS11Z		
10	500	50	EUFLS15Z		
15	2000	2000 20 <b>EUFLS</b>			
25	5000	20	EUFLS15M25		
75	10000	10	EUFLS110M75		


FLORISIL® A (100 / 120 Mesh) Florisil® is the trademark of U.S. Silica Co.

COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number	
3	500	50	EUFLSA153	
15	2000	20	EUFLSA12M15	

#### MECHANISM OF ION EXCHANGE BONDING

The retention mechanism in ion exchange bonding is the electrostatic attraction of the charged functional group on the compound to the charged functional group on the SPE sorbent. In order for an optimal interaction, both the compound of interest and the functional group on the bonded silica must be fully charged. To ensure 99% or more ionization, the pH should be at least two pH units below the pKa of the cation and two pH units above the pKa of the anion. Elution occurs by using a solution/buffer to raise the pH above the pKa of the cationic group or to lower the pH below the pKa of the anion to disrupt retention. At this point, the sorbent or compound is neutralized. Ion exchange resins come in two varying forms: strong and weak. The number of charges on a strong ion exchanger remains constant regardless of the buffer pH. Weak ion exchangers display pH-dependent functionality and therefore deliver optimal performance over only a small pH range.

Percent of Compound in Ionic State						
Functionality	Ionization	pH units away from pKa				
		2 < pKa	1 < pKa	At pKa	1 > pKa	2 > pKa
ACID	Anionic (-)	1	9	50	91	99
BASE	Cationic (+)	99	91	50	9	1

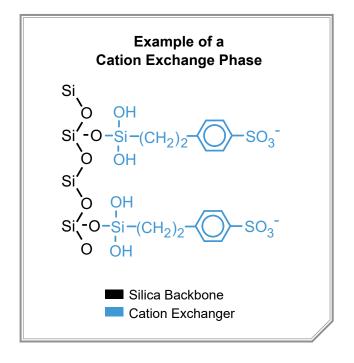

## **ION EXCHANGE SORBENTS & STRUCTURES**

Sorbent	Structure	рКа
Anion Exchangers		
NAX - Aminopropyl ( 1° amine )	-Si-(CH <sub>2</sub> ) <sub>3</sub> NH <sub>2</sub>	9.8
PSA - N-2 Aminoethyl ( 1° & 2° amine )	-Si-(CH <sub>2</sub> ) <sub>3</sub> NH(CH <sub>2</sub> ) <sub>2</sub> NH <sub>2</sub>	10.1, 10.9
DAX - Diethylamino (3° amine )	-Si-(CH <sub>2</sub> ) <sub>3</sub> N(CH <sub>2</sub> CH <sub>3</sub> ) <sub>2</sub>	10.6
EUQAX - Quaternary Amine Chloride	-Si-(CH <sub>2</sub> ) <sub>3</sub> N <sup>+</sup> (CH <sub>3</sub> ) <sub>3</sub> Cl <sup>-</sup>	Always charged
EHQAX - Quaternary Amine Hydroxide	-Si-(CH <sub>2</sub> )3N <sup>+</sup> (CH <sub>3</sub> ) <sub>3</sub> OH <sup>-</sup>	Always charged
EAQAX - Quaternary Amine Acetate	-Si-(CH <sub>2</sub> ) <sub>3</sub> N <sup>+</sup> (CH <sub>3</sub> ) <sub>3</sub> CH <sub>3</sub> COO <sup>-</sup>	Always charged
EFQAX - Quaternary Amine Formate	-Si-(CH <sub>2</sub> ) <sub>3</sub> N <sup>+</sup> (CH <sub>3</sub> ) <sub>3</sub> HCOO <sup>-</sup>	Always charged
PAX - Polyimine	-Si-(CH <sub>2</sub> ) <sub>3</sub> -R [NHCH <sub>3</sub> CH <sub>3</sub> ] <sub>x</sub>	
Cation Exchangers		
CCX - Carboxylic Acid	-Si-CH <sub>2</sub> COOH	4.8
PCX - Propylsulfonic Acid	-Si-(CH <sub>2</sub> ) <sub>3</sub> SO <sub>3</sub> H	<1
BCX - Benzenesulfonic Acid	-Si-(CH <sub>2</sub> ) <sub>2</sub> -\( \subseteq \sin \subseteq \subseteq \subseteq \subseteq \subseteq \subseteq \s	Always charged
BCXHL- Benzenesulfonic Acid High Load	-Si-(CH <sub>2</sub> ) <sub>2</sub> -\( \subseteq \subset	Always charged
TAX - Triacetic Acid	-Si-(CH <sub>2</sub> ) <sub>3</sub> NH-(CH <sub>2</sub> ) <sub>2</sub> N(CH <sub>2</sub> COOH) <sub>2</sub>	
	г СН <sub>2</sub> СООН	

	Goal	<b>Anion Exchange Sorbent</b>	Cation Exchange Sorbent
		рН	рН
WASH	To promote bonding between sorbent and analyte	> Analyte pKa and / or < Sorbent pKa	< Analyte pKa and / or > Sorbent pKa
ELUTION	To disrupt bonding between sorbent and analyte	< Analyte pKa and / or > Sorbent pKa	> Analyte pKa and / or < Sorbent pKa

## **ENVIRO-CLEAN®**

## **Anion Exchange Phase**

#### **AMINOPROPYL**

Organic Loading = 6.65% Surface Area = 500 m<sup>2</sup>/g Pore Volume = 0.77 cm<sup>3</sup>/g Average Pore Size = 60Å Anion Exchange = 0.28 meq/g

	COLUMNS				
Tube Volume (mL)	ume Sorbent Units p		Part Number		
3	200	50	EUNAX123		
3	500	50	EUNAX153		
6	500	50	EUNAX156		
6	1000	30	EUNAX1M6		
10	100	50	EUNAX11Z		
15	2000	20	EUNAX12M15		
75	10000	10	EUNAX110M75		

## QUATERNARY AMINE WITH CHLORIDE COUNTER ION

Organic Loading = 8.40%Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$  Average Pore Size = 60Å Anion Exchange = 0.230 meq/g

	COLUMNS			
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number	
1	100	100	EUQAX111	
3	200	50	EUQAX123	
3	500	50	EUQAX153	
6	500	50	EUQAX156	
6	1000	30	EUQAX1M6	
10	100	50	EUQAX11Z	
10	200	50	EUQAX12Z	
10	500	50	EUQAX15Z	

## QUATERNARY AMINE WITH ACETATE COUNTER ION

Organic Loading = 8.40%Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$  Average Pore Size = 60Å Anion Exchange = 0.230 meq/g

COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number	
3	500	50	EAQAX153	
6	1000	30	EAQAX1M6	
10	100	50	EAQAX11Z	
75	10000	10	EAQAX110M75	

## QUATERNARY AMINE WITH HYDROXIDE COUNTER ION


Organic Loading = 8.40%Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$  Average Pore Size = 60Å Anion Exchange = 0.230 meq/g

	COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number		
3	500	50	EHQAX153		
6	500	50	EHQAX156		

## QUATERNARY AMINE WITH FORMATE COUNTER ION

Organic Loading = 8.40%Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$  Average Pore Size = 60Å Anion Exchange = 0.230 meq/g

	COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number		
3	500	50	EFQAX153		
6	1000	30	EFQAX1M6		

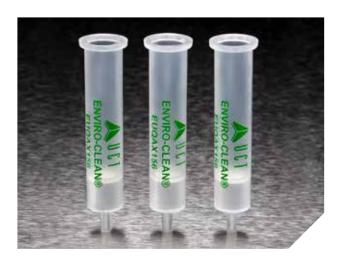

## **Anion Exchange Phase**



#### **POLYIMINE**

Organic Loading = 14.25%Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$  Average Pore Size = 60Å Anion Exchange = 0.880 meq/g

COLUMNS			
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number
3	500	50	EUPAX153
3	1000	50	EUPAX1M3
6	500	50	EUPAX156
6	1000	30	EUPAX1M6

#### PRIMARY/SECONDARY AMINE

Organic Loading = 11.1% Surface Area = 500 m<sup>2</sup>/g Pore Volume = 0.77 cm<sup>3</sup>/g Average Pore Size = 60Å Anion Exchange = 1.100 meq/g

	COLUMNS			
Tube Volume (mL)	Volume Sorbent Units per		Part Number	
1	50	100	EUPSA1L1	
1	100	100	EUPSA111	
3	200	50	EUPSA123	
3	500	50	EUPSA153	
6	500	50	EUPSA156	
6	1000	30	EUPSA1M6	
75	10000	10	EUPSA110M75	

## **ENVIRO-CLEAN®**

## Cation Exchange Phase

#### **CARBOXYLIC ACID**

Organic Loading = 8.75%Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$  Average Pore Size = 60Å Cation Exchange = 0.043 meq/g

	COLUMNS			
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number	
1	100	100	EUCCX111	
3	200	50	EUCCX123	
3	500	50	EUCCX153	
6	500	50	EUCCX156	
6	1000	30	EUCCX1M6	
10	200	50	EUCCX12Z	

#### **BENZENESULFONIC ACID**

Organic Loading = 10.69%Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$  Average Pore Size = 60Å Cation Exchange = 0.320 meq/g

	COLUMNS			
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number	
3	100	50	EUBCX113	
3	200	50	EUBCX123	
3	500	50	EUBCX153	
6	500	50	EUBCX156	
6	1000	30	EUBCX1M6	
10	100	50	EUBCX11Z	
10	200	50	EUBCX12Z	
10	500	50	EUBCX15Z	
15	2000	20	EUBCX12M15	
25	5000	20	EUBCX15M25	

#### TRIACETIC ACID

Organic Loading = 7.50% Surface Area = 500 m<sup>2</sup>/g Pore Volume = 0.77 cm<sup>3</sup>/g Average Pore Size = 60Å Cation Exchange = 0.10 meq/g Anion Exchange = 0.15 meq/g

	COLUMNS			
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number	
1	100	100	EUTAX111	
3	500	50	EUTAX153	
6	500	50	EUTAX156	
6	1000	30	EUTAX1M6	
10	100	50	EUTAX11Z	
75	10000	10	EUTAX110M75	

#### **BENZENESULFONIC ACID HIGH LOAD**

Organic Loading = 16.50%Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$  Average Pore Size = 60Å Cation Exchange = 0.650 meq/g

		COLUMNS	
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number
1	100	100	EUBCX1HL11
3	50	50	EUBCX1HLL3
3	100	50	EUBCX1HL13
6	500	50	EUBCX1HL56
6	1000	30	EUBCX1HLM6
10	200	50	EUBCX1HL2Z
10	500	50	EUBCX1HL5Z
75	10000	10	EUBCX1HL10M75

#### PROPYLSULFONIC ACID

Organic Loading = 7.00%Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$  Average Pore Size = 60Å Cation Exchange = 0.180 meq/g

	COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number		
3	500	50	EUPCX153		
10	500	50	EUPCX15Z		
15	2000	20	EUPCX12M15		

#### ENVIRO-CLEAN® COPOLYMERIC EXTRACTION SORBENTS

Copolymeric sorbents are composed of a silica backbone bonded with two types of functional chains. One is either an ion exchanger or polar chain, while the other is a hydrophobic carbon chain. The copolymeric phases manufactured by UCT are produced in a way as to allow for equal parts of each functional group to attach to the silica substrate yielding reproducible bonded phases and unique copolymeric chemistries. This type of mixed- mode seperation is beneficial when one is looking to extract both neutral and charged compounds and typically results in a cleaner, final extract.

www.unitedchem.com

## **ENVIRO-CLEAN®**

#### Copolymeric Exchange Phase

Sorbent	Category	Structure	рКа
Benzenesulfonic Acid (BCX2)	Strong Cation	C8 + -Si-(CH2)2-Ph-SO3-	Always Charged
Benzenesulfonic Acid (BCX3)	Strong Cation	C18 + -Si-(CH2)2-Ph-SO3-	Always Charged
Propylsulfonic Acid (PCX2)	Strong Cation	C8 + -Si-(CH2)3SO3H	<1
Carboxylic Acid (CCX2)	Weak Cation	C8 + -Si-(CH2)2COOH	4.8
Quaternary Amine (QAX2)	Strong Anion	C8 + -Si-(CH2)3N + (CH3)3	Always Charged
Quaternary Amine (QAX3)	Strong Anion	C18 + -Si-(CH2)3N + (CH3)3	Always Charged
Aminopropyl (NAX2)	Weak Anion	C8 + -Si-(CH2)3NH2	9.8
Cyanopropyl (CNP2)	Hydrophilic	C8 + -Si-(CH2)3CN	N/A
Cyclohexyl (CYH2)	Hydrophobic	C8 + -Si-(CH2)-C6H12	N/A


Analytes	Washes	Elutions	
Cations/Anions	1) Aqueous to remove polar matrix components.	1) Organic to elute hydrophobically bound analytes.	
Alkanes	2) Methanol to disrupt residual hydrophobic	2) Organic with a pH that would	
Alkenes	interferences and to remove any remaining residual matrix.	neutralize ionically bound analytes.	
Aromatics		3) Aqueous buffer with high ionic strength.	
		4) Solvent possessing a counter ion that would bond to sorbent and displace analyte of interest.	


#### **EXTRACTION MECHANISMS OF COPOLYMERIC BONDED PHASES**


A sample composed of a theoretical neutral parent drug and its charged (acidic) metabolite is applied at a pH of 6 (**Figure 1**). At this pH, most amine groups are positively charged. Since this sorbent is positively charged, compounds with positively charged cations are repelled. Depending on the pKa of the metabolite, the carboxylic acid groups may be negatively charged, allowing the metabolite to bond to the positively charged sorbent. The column also possesses a hydrophobic chain which allows the neutral parent drug to bond to the sorbent.


Water or a weak aqueous buffer (pH 6) washes away hydrophilically bound interferences (**Figure 2**). The column is then dried utilizing organic solvent to ensure it's free of any residual aqueous phase that would hinder effective elution.

After drying, analytes of interest can be eluted using a two-step process. During the first elution (Figure 3), the hydrophobically bound neutral parent drug is eluted with a solvent of minimal polarity, such as hexane/ethyl acetate (80:20). The second elution (Figure 4) employs an acid to neutralize the charge of acidic analytes. The ionic interaction is released, and analytes are eluted in an appropriate solvent mixture. If a tiered elution scheme is not desired, a universal solvent can be put to use that can effectively disrupt both bonding mechanisms at once to elute all analytes of interest within one single elution step.

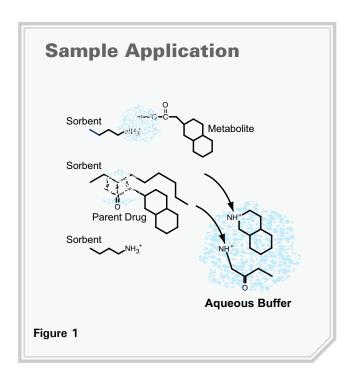

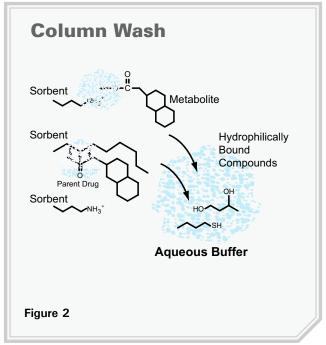

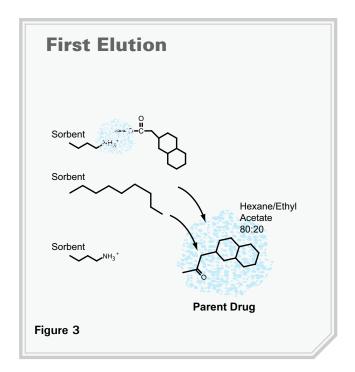

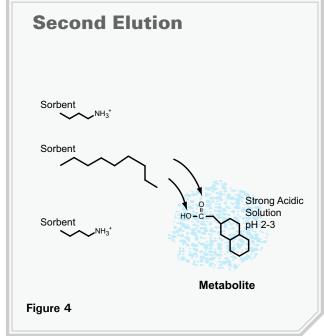

## **ENVIRO-CLEAN®**

## Copolymeric Exchange Phase

#### **C8 PLUS CYCLOHEXYL**

Organic Loading = 14.0% Surface Area = 500 m<sup>2</sup>/g

Average Pore Size = 60Å Pore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

	COLUMNS					
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number			
3	200	50	EUCYH223			
6	500	50	EUCYH256			

#### **C8 PLUS CYANOPROPYL**

Organic Loading = 14.0% Surface Area = 500 m<sup>2</sup>/g

Average Pore Size = 60Å Pore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

COLUMNS					
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number		
3	200	50	EUCNP223		

#### **C8 PLUS PROPYLSULFONIC**

Organic Loading = 14.62% Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

Average Pore Size = 60Å Exchange Capacity = 0.11 meq/g

	COLUMNS					
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number			
3	200	50	EUPCX223			
6	500	50	EUPCX256			

#### **C8 PLUS CARBOXYLIC ACID**

Organic Loading = 11.45% Surface Area =  $500 \text{ m}^2/\text{g}$ 

Average Pore Size = 60Å Exchange Capacity = 0.110 meq/g

Pore Volume =  $0.77 \text{ cm}^3/\text{g}$ 

COLUMNS					
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number		
3	200	50	EUCCX223		
6	1000	30	EUCCX2M6		
10	200	50	EUCCX22Z		



## Copolymeric Exchange Phase



#### **C8 PLUS BENZENESULFONIC ACID**

Organic Loading = 12.40% Surface Area = 500 m<sup>2</sup>/g Pore Volume = 0.77 cm<sup>3</sup>/g Average Pore Size = 60Å
Exchange Capacity = 0.077 meq/g

	COLUMNS					
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number			
3	200	50	EUBCX223			
6	500	50	EUBCX256			
6	1000	30	EUBCX2M6			
10	200	50	EUBCX22Z			
10	500	50	EUBCX25Z			

#### C18 PLUS BENZENESULFONIC ACID

Organic Loading = 12.4%Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$  Average Pore Size = 60Å Exchange Capacity = 0.077 meq/g

	COLUMNS					
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number			
3	50	50	EUBCX3L3			
3	100	50	EUBCX313			

#### **C8 PLUS AMINOPROPYL**

Organic Loading = 12.10% Surface Area =  $500 \text{ m}^2/\text{g}$ Pore Volume =  $0.77 \text{ cm}^3/\text{g}$  Average Pore Size = 60Å Exchange Capacity = 0.144 meq/g

	COLUMNS				
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number		
3	200	50	EUNAX223		
3	500	50	EUNAX253		
6	1000	30	EUNAX2M6		
10	100	50	EUNAX21Z		
75	1000	10	EUNAX10M75		

#### **C8 PLUS QUATERNARY AMINE**

Organic Loading = 13.00% Surface Area = 500 m<sup>2</sup>/g Pore Volume = 0.77 cm<sup>3</sup>/g Average Pore Size = 60Å Exchange Capacity = 0.170 meq/g

COLUMNS					
Tube Volume (mL)	Sorbent Amount (mg)	Units per Pack	Part Number		
3	200	50	EUQAX223		
3	500	50	EUQAX253		
6	500	50	EUQAX256		
6	1000	30	EUQAX2M6		

### **ENVIRO-CLEAN®** Polymeric DVB Extraction Sorbent



Enviro-Clean® polymeric extraction sorbents are formulated with an ultra-clean, highly cross-linked styrene and divinylbenzene polymer sorbent. The sorbent can be functionalized with many of the same phases as our silica based sorbents. Possibilities include standard ion exchange functionalities. Enviro-Clean® particles have an average particle size of 30 microns with enhanced loading capacity. This higher capacity translates into lower requirements for bed mass. The Enviro-Clean® sorbent also eliminates the need for the initial column conditioning step. All of these attributes ultimately result in improved cost to the end user.

### Advantages of ENVIRO-CLEAN® DVB Sorbent:

- No conditioning steps
- High and reproducible recoveries
- Cross-linked sorbent minimized bead swelling
- Reduced sorbent mass
- Improved flow rates
- pH stable from 1-14
- High sorbent capacity

		COLUMNS		
Tube Volume (mL)	Sorbent Amount (mg)	Frit Type	Units per Pack	Part Number
3	50	PTFE	50	ECDVB1L3
3	60	PE	100	ECDVB063P
3	100	PTFE	50	ECDVB113
3	100	PTFE	500	ECDVB113-D
6	200	PE	30	ECDVB126P
6	500	PTFE	30	ECDVB156
6	500	PE	30	ECDVB156P
15	1000	PTFE	20	ECDVB1M15

## **ENVIRO-CLEAN®** Inert Glass Cartridge

For ultra-clean extractions, UCT offers inert, 6 mL glass cartridges in a variety of bonded phases packed between two PTFE frits.




COLUMNS					
Tube Volume (mL)	Sorbent Amount (mg)	Bonded Phase	Endcapped	Units per Pack	Part Number
6	500	C2-ETHYL	YES	100	EEC02156G
6	500	C8-OCTYL	YES	50	EEC08156G
6	500	C18-OCTADECYL	NO	50	EUC18156G
6	500	C18-OCTADECYL	YES	50	EEC18156G
6	1000	C18-OCTADECYL	NO	30	EUC181M6G
6	1000	C18-OCTADECYL	YES	50	EEC181M6G
6	1000	CYCLOHEXL	YES	50	EECYH1M6G
6	1000	PHENYL	NO	50	EUPHY1M6G
6	1000	ALUMINA-NEUTRAL	N/A	30	EUALN1M6G
6	500	SILICA-ACID WASHED	N/A	10	EUSIL156G
6	1000	SILICA-ACID WASHED	N/A	10	EUSIL1M6G
6	500	PHARMA-SIL® SILICA	N/A	10	EPHSIL156G
6	200	POLYSTYRENE DVB	N/A	10	ECDVB126G
6	500	POLYSTYRENE DVB	N/A	10	ECDVB156G

## ENVIRO-CLEAN® BULK SORBENT GUIDE





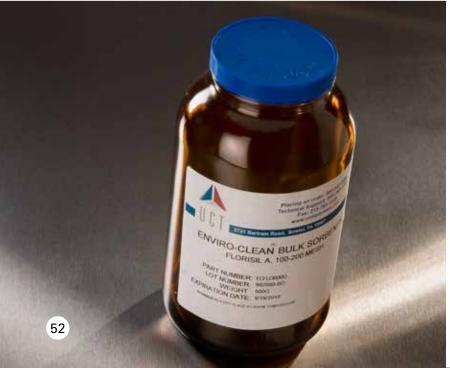





UCT sorbents are available in bulk quantities in a variety of sizes ranging from 10g to 50Kg. Common bulk sorbents used in environmental analysis are listed below, but all varities of bonded phases can be packaged in comparable quantities.

PRODUCT NAME	PART NUMBER	QUANTITY
0	ECCU01K	1kg
Copper Granules 99.5% 30 Mesh	ECCU05K	5kg
SO Mesti	ECCU10K	10kg
Alumina	ECALN00D	500g
Activity Super I, Neutral	ECALN01K	1kg
Activity Super i, Neutral	ECALN03K	3kg
Alumina	ECALB00D	500g
Activity Super I, Basic	ECALB01K	1kg
Activity Super 1, Busic	ECALB03K	3kg
Alumina	ECALA00D	500g
Activity Super I, Acid	ECALA01K	1kg
Florisil® A	ECFLOR00D	500g
100-200 Mesh	ECFLOR03K	3kg
	ECFLS00X	10g
Florisil® PR	ECFLS00D	500g
	ECFLS03K	3kg
Silica Gel	ECSIOH00D	500g
100-200 Mesh suitable for column chromatography	ECSIOH03K	3kg
	ECSS01K	1kg
Sodium Sulfate	ECSS05K	5kg
Anhydrous	ECSS10K	10kg
ACS Grade Granular 60 Mesh	ECSS25K	25kg
	ECSS50K	50kg (Sent as 2 x 25kg)
Magnesium Sulfate	ECMAG00C	100g (1 unit)
Anhydrous Organic Free	ECMAG00D	500g (1 unit)
Powder Reagent, 99.5% min.	ECMAG00DCS	1 case (4 units)
0-14- 500	EC56601K	1kg
Celite 566 Hydromatrix Substitute	EC56603K	3kg
Trydromatrix Substitute	EC566030K	30kg
	ECOTT01K	1kg
Out-out-Cond	ECOTT05K	5kg
Ottawa Sand	ECOTT10K	10kg
	ECOTT25K	25kg
Graphitized Carbon	EUCARB00C	100g
120/400 Mesh	EUCARB00K	1kg

## MANIFOLDS



## **Disk Manifold and Accessories**



6 Station Manifold



Bottle Holder



Universal Cartridge Adapter



90mm Aluminum Clamp



90mm Support Base



90mm 1000ml Funnel



Vacuum Pump



Waste Trap



Glass Cartridge Adapter



Jar Holder



47mm Aluminum Clamp




47mm Support Base



47mm 300ml Funnel



47mm/90mm KEL-F Screen



Teflon Stopcock and Body

Description	Units	Part Number
Manifolds		
1 Station Manifold	1	ECUCTVAC1
3 Station Manifold	1	ECUCTVAC3
6 Station Manifold	1	ECUCTVAC6
NOTE: The above numbers indicate the stainless steel	manifolds ba	ase only.
UCT Universal Cartridge Accessories		
Glass cartridge adapter	1	ECUCTADP
Universal cartridge bottle holder adapter	1	ECUNIBHD
Universal cartridge jar bottle holder adapter	1	ECUNIJHD100
Universal cartridge adapter	1	ECBMADP
(Compatible with JT Baker Manifold*)		
SPE Disk Accessories		
47mm aluminum clamp	1	ECCG1420
90mm aluminum clamp	1	ECUC0502
47mm support base	1	ECQSB47
90mm support base	1	ECQSB90
47mm 300 mL funnel	1	ECQFN300
90mm 1000 mL funnel	1	ECQFN1000
47mm KEL-F screen	1	ECUCT47
90mm KEL-F screen	1	ECUCT90
Additional Accessories		
Vacuum pump - 110 volt	1	ECROCKER400
Vacuum pump - 220 volt	1	ECROCKER400-220
Teflon stopcock and body	1	ECUCTSC
Waste trap	1	ECUCTTRAP20

#### **GLASS BLOCK MANIFOLD**


A complete Vacuum Manifold System consists of a glass block, Corian® manifold lid, a cover gasket, vacuum gauge and assembly, PTFE tips, an adjustable collection rack, bulkhead luer fittings, plugs and a glass block safety tray. The Vacuum Manifold System is available in either 16 or 24 positions. These manifold systems are durable and highly chemical resistant, designed to provide years of trouble-free extractions.




Description	Part Number
Complete 16 Position Vacuum Manifold System	VMF016GL
Complete 24 Position Vacuum Manifold System	VMF024GL

## **GLASS BLOCK MANIFOLD ACCESSORIES**









Manifold Lid (16 Position)





(24 Position)

Manifold Lid



Manifold Lid Legs

Gasket

Collection Rack







Collection Rack (12 Position) Collection Rack Posts



Collection Rack

Retaining Clips

Vacuum Gauge and Bleed Valve





**Bulkhead Luer Fittings** 

Luer Plugs





Flange Caps

Large Volume Transfer Tubes





20L Waste Trap

Description	Units	Part Number
Manifold Lid (16 position) – A rigid Corian® lid which resists warping with extended use. Lids come with caps, bulkhead fittings and gasket.	1	VMF06120
<b>Manifold Lid (24 position)</b> – A rigid Corian® lid which resists warping with extended use. Lids come with caps, bulkhead fittings and gasket.	1	VMF04120
Manifold Lid Legs – The lid legs can be used to set the manifold lid on a surface while loading columns, changing collection tubes or removing waste.	4	VMF02120-1
<b>Gasket</b> – A foam gasket that fits both the 16 and 24 position lids.	2	VMF04121
Collection Rack (16 position) – A polypropylene rack that is highly resistant to chemical degradation and abuse. This rack allows the use of 13 and 16 mm disposable test tubes.	1	VMF06125
<b>Collection Rack (24 position)</b> – A polypropylene rack that is highly resistant to chemical degradation and abuse. This rack allows the use of 13 and 16 mm disposable test tubes.	1	VMF04125
Collection Rack (12 position) – A polypropylene rack that is highly resistant to chemical degradation and abuse. This rack is designed for the use of 27 mm (VOA vials) and smaller disposable collection vials.	1	VMF02125
<b>Collection Rack Posts</b> – These posts can be ordered as replacements parts for the posts in all collection racks.	3	VMF02127
Collection Rack Retaining Clips – These clips are replacement parts for the clips included in all collection racks.	12	VMF02129
<b>Vacuum Gauge and Bleed Valve</b> – This system is used in monitoring and adjusting vacuum.	1	VMF02122
<b>Bulkhead Luer Fittings</b> – These fittings screw into the lid allowing the sample to transfer from the column into the PTFE Luer tip to the test tube.	12	VMF21BFN
<b>Luer Plugs</b> – These plugs fit into the bulkhead fittings in order to seal unused bulkhead fittings. These can also be used to break vacuum to the manifold.	12	VMF21PLN
1 mL 3 mL Flange Caps – Used with the Luer Caps, Flange Caps plug the top of SPE cartridges. 15 mL 25 mL	50 50 50 50 50	CR0001P CR0004P CR0008P CR0015P CR0025P
<b>Large Volume Transfer Tubes</b> – Used to transfer large volumes (100-1000mL) from a water collection bottle to an SPE cartridge.	6 12	VMFSTFR06 VMFSTFR12
Large Volume Transfer Tubes For Perfluorinated Compound Analysis – Used to transfer large volumes (100-1000mL) from a water collection bottle to an SPE cartridge.	6 12	VMFSTFR06 - PFC VMFSTFR12 - PFC
1, 3, 6, 10 mL Cartridge Adapters	15 100	AD0000AS AD00000C
20L Waste Trap	1	ECUCTTRAP20
<b>20L Waste Trap Adapter</b> – 3/8" x 1/4" PVDF ADPT for fitting to glass block manifold.	1	ECUCTTRAP20-ADPT



## SELECTRA® U/HPLC COLUMNS





The SELECTRA® line of HPLC columns is created using an ultra-high purity, Type B, spherical silica. This support material minimizes surface activity and allows for high density functional group bonding.

Columns are available with either 1.8, 3, or 5 µm particle sizes.

Guard Column Holder				
Description	Part Number			
HPLC Guard Cartridge Holder	SLGRDHLDR			
UHPLC Direct Connect Guard Cartridge Holder	SLGRDHLDR-HPOPT			
Replacement Peek Tip for Holder	SLGRDHLDR-TIP (2/pk)			

#### **SELECTRA® DA**

- Unique Biphenyl phase.
- Excellent selectivity for a wide range of compounds including therapeutic drugs, drugs of abuse, mycotoxins, veterinary drugs and pesticides.
- Ability to retain compounds that can be difficult to retain on a C18
- Can achieve significant selectivity changes with the choice of acetonitrile or methanol as the organic solvent.
- Carbon Load 13%.
- Conforms to USP L11.
- Fully endcapped.

SELECTRA® DA					
Column Length (mm)	Column i.d. (mm)	Particle Size	Part Number		
50	2.1	1.8 µm	SLDA50ID21-18UM		
100	2.1	1.8 µm	SLDA100ID21-18UM		
50	4.6	1.8 µm	SLDA50ID46-18UM		
100	4.6	1.8 µm	SLDA100ID46-18UM		
50	2.1	3 µm	SLDA50ID21-3UM		
100	2.1	3 µm	SLDA100ID21-3UM		
50	4.6	3 µm	SLDA50ID46-3UM		
100	4.6	3 µm	SLDA100ID46-3UM		
150	4.6	3 µm	SLDA150ID46-3UM		
50	2.1	5 µm	SLDA50ID21-5UM		
100	2.1	5 µm	SLDA100ID21-5UM		
50	4.6	5 µm	SLDA50ID46-5UM		
100	4.6	5 µm	SLDA100ID46-5UM		
150	4.6	5 µm	SLDA150ID46-5UM		
250	4.6	5 µm	SLDA250ID46-5UM		

	<b>Guard Cartridge</b>	Columns	(2/pack)*
10	2.0	1.8 µm	SLDAGDC20-18UMOPT
10	2.0	3 µm	SLDAGDC21-3UM
10	2.0	5 µm	SLDAGDC21-5UM
10	4.6	1.8 µm	SLDAGDC46-18UMOPT
10	4.6	3 µm	SLDAGDC46-3UM
10	4.6	5 µm	SLDAGDC46-5UM

<sup>\*</sup>Guard Cartridge columns must be used with a UCT guard cartridge holder.

#### **Storage of LC Columns:**

Do not allow LC analytical columns to stand uncapped for any length of time. Store an LC column in methanol or an appropriate organic solvent, capped at both ends. A dry LC column is sometimes difficult to reactivate and may not recover to full performance status.

## SELECTRA® U/HPLC Columns

#### SELECTRA® C18

- Optimum retention for traditional reverse phase analysis.
- Highest hydrophobic interactions in the Selectra® column line.
- Carbon Load 20%.
- Conforms to USP L1.
- · Fully endcapped.



#### SELECTRA® Aqueous C18

- Polar modified C18.
- Similar non-polar retention to traditional C18.
- Enhanced selectivity and retention for difficult to retain polar analytes.
- Suitable in up to 100% aqueous mobile phases.
- Carbon Load 10%.
- Conforms to USP L1.
- Fully endcapped.

	SELECT	RA® C18	
Column Length (mm)	Column i.d. (mm)		Part Number
50	2.1	1.8 µm	SLC-1850ID21-18UM
100	2.1	1.8 µm	SLC-18100ID21-18UM
50	4.6	1.8 µm	SLC-1850ID46-18UM
100	4.6	1.8 µm	SLC-18100ID46-18UM
50	2.1	3 µm	SLC-1850ID21-3UM
100	2.1	3 µm	SLC-18100ID21-3UM
50	4.6	3 µm	SLC-1850ID46-3UM
100	4.6	3 µm	SLC-18100ID46-3UM
150	4.6	3 µm	SLC-18150ID46-3UM
50	2.1	5 µm	SLC-1850ID21-5UM
100	2.1	5 μm	SLC-18100ID21-5UM
50	4.6	5 µm	SLC-1850ID46-5UM
100	4.6	5 µm	SLC-18100ID46-5UM
150	4.6	5 µm	SLC-18150ID46-5UM
250	4.6	5 μm	SLC-18250ID46-5UM
Gua	ard Cartridge	Columns (2	2/pack)*
10	2.0	1.8 µm <b>S</b> I	LC-18GDC20-18UMOPT
10	2.0	3 µm	SLC-18GDC20-3UM
10	2.0	5 µm	SLC-18GDC20-5UM
10	4.6	1.8 µm <b>SL</b>	.C-18GDC46-18UMOPT
10	4.6	3 µm	SLC-18GDC46-3UM
10	4.6	5 µm	SLC-18GDC46-5UM

\*Guard Cartridge columns must be used with a UCT guard cartridge holder.

	SELECTRA® A	Aqueous	C18
Column Length (mm)	Column i.d. (mm)	Particle Size	Part Number
50	2.1	1.8 µm	SLAQ50ID21-18UM
100	2.1	1.8 µm	SLAQ100ID21-18UM
50	4.6	1.8 µm	SLAQ50ID46-18UM
100	4.6	1.8 µm	SLAQ100ID46-18UM
50	2.1	3 µm	SLAQ50ID21-3UM
100	2.1	3 µm	SLAQ100ID21-3UM
50	4.6	3 µm	SLAQ50ID46-3UM
100	4.6	3 µm	SLAQ100ID46-3UM
150	4.6	3 µm	SLAQ150ID46-3UM
50	2.1	5 µm	SLAQ50ID21-5UM
100	2.1	5 µm	SLAQ100ID21-5UM
50	4.6	5 µm	SLAQ50ID46-5UM
100	4.6	5 µm	SLAQ100ID46-5UM
150	4.6	5 µm	SLAQ150ID46-5UM
250	4.6	5 µm	SLAQ250ID46-5UM
Gua	ard Cartridge C	olumns (	2/pack)*
10	2.0	1.8	SLAQGDC20-18UMOPT
10	2.0	3	SLAQGDC20-3UM
10	2.0	5	SLAQGDC20-5UM
10	4.6	1.8	SLAQGDC46-18UMOPT
10	4.6	3	SLAQGDC46-3UM
10	4.6	5	SLAQGDC46-5UM

<sup>\*</sup>Guard Cartridge columns must be used with a UCT guard cartridge holder.

SELECTRA® PFPP					
Column Length (mm)	Column i.d. (mm)	Particle Size	Part Number		
50	2.1	1.8 µm	SLPFPP50ID21-18UM		
100	2.1	1.8 µm	SLPFPP100ID21-18UM		
50	4.6	1.8 µm	SLPFPP50ID46-18UM		
100	4.6	1.8 µm	SLPFPP100ID46-18UM		
50	2.1	3 µm	SLPFPP50ID21-3UM		
100	2.1	3 µm	SLPFPP100ID21-3UM		
50	4.6	3 µm	SLPFPP50ID46-3UM		
100	4.6	3 µm	SLPFPP100ID46-3UM		
150	4.6	3 µm	SLPFPP150ID46-3UM		
50	2.1	5 µm	SLPFPP50ID21-5UM		
100	2.1	5 µm	SLPFPP100ID21-5UM		
50	4.6	5 µm	SLPFPP50ID46-5UM		
100	4.6	5 µm	SLPFPP100ID46-5UM		
150	4.6	5 µm	SLPFPP150ID46-5UM		
250	4.6	5 µm	SLPFPP250ID46-5UM		
Guard Cartridge Columns (2/pack)*					

	<b>Guard Cartridge</b>	Columns	s (2/pack)*
10	2.0	1.8 µm	SLPFPPGDC20-18UMOPT
10	2.0	3 µm	SLPFPPGDC20-3UM
10	2.0	5 µm	SLPFPPGDC20-5UM
10	4.6	1.8 µm	SLPFPPGDC46-18UMOPT
10	4.6	3 µm	SLPFPPGDC46-3UM
10	4.6	5 µm	SLPFPPGDC46-5UM

<sup>\*</sup>Guard Cartridge columns must be used with a UCT guard cartridge holder.

SELECTRA® C8						
Column Length (mm)	Column i.d. (mm)	Particle Size	Part Number			
50	2.1	1.8 µm	SLC-850ID21-18UM			
100	2.1	1.8 µm	SLC-8100ID21-18UM			
50	4.6	1.8 µm	SLC-850ID46-18UM			
100	4.6	1.8 µm	SLC-8100ID46-18UM			
50	2.1	3 µm	SLC-850ID21-3UM			
100	2.1	3 µm	SLC-8100ID21-3UM			
50	4.6	3 µm	SLC-850ID46-3UM			
100	4.6	3 µm	SLC-8100ID46-3UM			
150	4.6	3 µm	SLC-8150ID46-3UM			
50	2.1	5 µm	SLC-850ID21-5UM			
100	2.1	5 µm	SLC-8100ID46-5UM			
50	4.6	5 µm	SLC-850ID46-5UM			
100	4.6	5 µm	SLC-8100ID46-5UM			
150	4.6	5 µm	SLC-8150ID46-5UM			
250	4.6	5 μm	SLC-8250ID46-5UM			
Gua	ard Cartridge (	Columns	(2/pack)*			
10	2.1	1.8 µm	SLC-8GDC21-18UMOPT			
10	2.1	3 µm	SLC-8GDC21-3UM			
10	2.1	5 µm	SLC-8GDC21-5UM			
10	4.6	1.8 µm	SLC-8GDC46-18UMOPT			
10	4.6	3 µm	SLC-8GDC46-3UM			
10	4.6	5 µm	SLC-8GDC46-5UM			

<sup>\*</sup>Guard Cartridge columns must be used with a UCT guard cartridge holder.

#### SELECTRA® PFPP

- Can be used for reverse phase, normal phase, or HILIC separations.
- Exhibits multiple selectivity
  mechanisms including hydrogen
  bonding, dipole dipole, pi-pi over
  lap, hydrophilic (HILIC), and hy
  drophobic interactions.
- Carbon Load 11%.
- Conforms to USP L43.
- Fully endcapped.



#### **SELECTRA®** C8

- Less retentive, less hydrophobic than standard C18 column.
- Selectivity similar to C18 for non-polar compounds.
- Carbon Load 12%.
- Conforms to USP L7.
- Fully endcapped.

# ACCESSORIES

GC LINERS **RESERVOIRS FRITS** 62



Gas Chromatograph Glass Liners manufactured by UCT are deactivated using a proprietary silane. The silane is manufactured by UCT Specialties, LLC, a leader in high purity, specialty silanes for the chromatographic industry.

DESCRIPTION	INNER DIAMETER (mm)	OUTER DIAMETER (mm)	LENGTH (mm)	INSTRUMENT	UNITS	UCT Part Number
2 mm Straight Split/Splitless	2.0	6.5	78.5	Agilent	1 5 25	GCL2MM GCL2MM-5 GCL2MM-25
2 mm Straight Split/Splitless with Deactivated Glass Wool	2.0	6.5	78.5	Agilent	1 5 25	GCL2MMGW GCL2MMGW-5 GCL2MMGW-25
2 mm Gooseneck Split/Splitless	2.0	6.5	78.5	Agilent	1 5 25	GCLGN2MM GCLGN2MM-5 GCLGN2MM-25
2 mm Gooseneck Split/Splitless with Deactivated Glass Wool	2.0	6.5	78.5	Agilent	1 5 25	GCLGN2MMGW-5 GCLGN2MMGW-5 GCLGN2MMGW-25
4 mm Straight Split/Splitless	4.0	6.5	78.5	Agilent	1 5 25	GCL4MM GCL4MM-5 GCL4MM-25
4 mm Straight Split/Splitless with Deactivated Glass Wool	4.0	6.5	78.5	Agilent	1 5 25	GCL4MMGW-5 GCL4MMGW-25
4 mm Recessed Gooseneck Split/Split- less	4.0	6.5	78.5	Agilent	1 5 25	GCLRG4MM GCLRG4MM-5 GCLRG4MM-25
4 mm Recessed Gooseneck Split/Split- less with Deactivated Glass Wool	4.0	6.5	78.5	Agilent	1 5 25	GCLRG4MMGW-5 GCLRG4MMGW-25
4 mm Gooseneck Split/Splitless	4.0	6.5	78.5	Agilent	1 5 25	GCLGN4MM GCLGN4MM-5 GCLGN4MM-25
4 mm Gooseneck Split/Splitless with Deactivated Glass Wool	4.0	6.5	78.5	Agilent	1 5 25	GCLGN4MMGW-5 GCLGN4MMGW-25
3.4 mm Straight Split 1078/1079 Inlet	3.4	5.0	54	Varian/ Bruker	1 5 25	GCL3.4MM GCL3.4MM-5 GCL3.4MM-25
3.4 mm Straight Split with Frit Inserted 1078/1079 Inlet	3.4	5.0	54	Varian/ Bruker	1 5 25	GCL3.4MMFR GCL3.4MMFR-5 GCL3.4MMFR-25

## Reservoirs





	POL	YPROPYLEN	E RESERVOIRS	
Volume Capacity	Units per Pack	No. of Frits	Porosity of Frits (µm)	Part Number
1 mL	50	0	N/A	RFV0001P
1 mL	50	1	10	RFV01F1P
1 mL	50	2	10	RFV02F1P
1 mL	50	1	20	RFT01F1P
1 mL	50	2	20	RFT02F1P
4 mL	50	0	N/A	RFV0004P
4 mL	50	1	10	RFV01F4P
4 mL	50	2	10	RFV02F4P
4 mL	50	1	20	RFT01F4P
4 mL	50	2	20	RFT02F4P
8 mL	50	0	N/A	RFV0008P
8 mL	50	1	10	RFV01F8P
8 mL	50	2	10	RFV02F8P
8 mL	50	1	20	RFT01F8P
8 mL	50	2	20	RFT02F8P
10 mL	50	0	N/A	RFV0010P
10 mL	50	1	10	RFV1F10P
10 mL	50	2	10	RFV2F10P
10 mL	50	1	20	RFT1F10P
10 mL	50	2	20	RFT2F10P
15 mL	50	0	N/A	RFV0015P
15 mL	50	1	10	RFV1F15P
15 mL	50	2	10	RFV2F15P
15 mL	50	1	20	RFT1F15P
15 mL	50	2	20	RFT2F15P
25 mL	50	0	N/A	RFV0025P
25 mL	50	1	10	RFV1F25P
25 mL	50	2	10	RFV2F25P
25 mL	50	1	20	RFT1F25P
25 mL	50	2	20	RFT2F25P
75 mL	50	0	N/A	RFV0075P
75 mL	50	1	10	RFV1F75P
75 mL	50	2	10	RFV2F75P
75 mL	50	1	20	RFT1F75P
75 mL	50	2	20	RFT2F75P
150 mL	10	0	N/A	RFV00150P
150 mL	10	1	20	RFT1F150P
150 mL	10	2	20	RFT2F150P



FLANGELESS POLYPROPYLENE RESERVOIRS					
Volume Capacity	Units per Pack	No. of Frits	Porosity of Frits (µm)	Part Number	
4 mL	50	0	N/A	RFT00R3P	
4 mL	50	1	20	RFT1FR3P	
10 mL	50	1	20	RFT1FR10P	



GLASS RESERVOIRS					
Volume Capacity	Units per Pack	No. of Frits	Porosity of Frits (µm)	Part Number	
8 mL	30	0	N/A	RFV0008G	
8 mL	30	1	10	RFV01F8G	



48 DEEP WELL FILTER PLATES						
Description Part Number Units						
Empty 48 deep well plate with one frit inserted	WIM481F	1				
Loose 48 deep well plate square frits	FR10481P	48				
48 deep well collection plate	WIM48CP	1				





96 DEEP WELL FILTER PLATES						
Description	Part Number	Units				
Empty 96 deep well plate with one frit inserted	WSH961FR	1				
Loose 96 deep well plate square frits	FRSH2096P	96				
96 well collection plate	WSH96CP	1				
96 well plate sealable lid	WSH96PS	1				





POLYPROPYLENE CARTRIDGES					
Volume Capacity	Units per Pack	No. of Frits	Porosity of Frits (µm)	Part Number	
600 mg (Medium)	50	0	N/A	RFV000MC	
600 mg (Medium)	50	2	20	RFT02FMC	
900 mg (Large)	50	0	N/A	RFV000LC	
900 mg (Large)	50	2	20	RFT02FLC	



POLYETHYLENE FRITS					
Column Size	Diameter	Porosity	Thickness	Units	Part Number
1 mL	0.232"	10 µm	1/16"	100	FR10011P
1 mL	0.232"	20 µm	1/16"	100	FR20011P
1 mL	0.232"	20 µm	1/8"	100	FT20011P
4 mL	0.357"	7 μm	1/16"	100	FR07041P
4 mL	0.357"	10 µm	1/16"	100	FR10041P
4 mL	0.357"	20 µm	1/16"	100	FR20041P
4 mL	0.357"	20 µm	1/8"	100	FT20041P
4 mL	0.357"	100 µm	1/16"	100	FR100041P
8 mL	0.498"	10 µm	1/16"	100	FR10081P
8 mL	0.498"	20 µm	1/16"	100	FR20081P
8 mL	0.513"	20 µm	1/8"	100	FT20081P
10 mL	0.357"	10 µm	1/16"	100	FR10101P
10 mL	0.357"	20 µm	1/16"	100	FR20101P
10 mL	0.357"	20 µm	1/8"	100	FT20101P
15 mL	0.630"	10 µm	1/16"	100	FR10151P
15 mL	0.641"	20 µm	1/16"	100	FR20151P
15 mL	0.641"	20 µm	1/8"	100	FT20151P
25 mL	0.792"	10 µm	1/16"	100	FR10251P
25 mL	0.792"	20 µm	1/16"	100	FR20251P
25 mL	0.816"	20 µm	1/8"	100	FT20251P
75 mL	1.050"	10 µm	1/16"	100	FR10751P
75 mL	1.050"	20 μm	1/16"	100	FR20751P
75 mL	1.050"	20 μm	1/8"	100	FT20751P
150 mL	1.515"	20 μm	1/16"	20	FR201501P
150 mL	1.515"	20 μm	1/8"	20	FT201501P
		PT	FE FRITS		
Column Size	Diameter	Porosity	Thickness	Units	Part Number

PTFE FRITS						
Column Size	Diameter	Porosity	Thickness	Units	Part Number	
4 mL	0.357"	10 μm	1.5 mm	60	FR10041T	
8 mL	0.498"	10 μm	1.5 mm	60	FR10081T	
8 mL	0.498"	50 μm	1.5 mm	60	FR50081T	
15 mL	0.641"	10 µm	1.5 mm	60	FR10151T	
15 mL	0.641"	50 μm	1.5 mm	100	FR50151T	





#### **PRICES AND TERMS**

Our prices are subject to change without notice. The price in effect when we receive your order will apply. All prices are in US Dollars and are shipped F.O.B. Terms of payment are net 30 days.

#### MINIMUM ORDERS\*

We welcome all orders, therefore, we do not have a minimum order requirement. When ordering, please include your purchase order number, complete "Ship To" and "Bill To" address, catalog number, quantity, and description of product(s). Also include your name and a phone number where you can be reached should we have any questions concerning your order.

\*Custom items will be evaluated on an individual basis; quantity requirements may be necessary.

#### **SHIPMENTS**

Normal processing is within 24-48 hours after receipt of an order. Unless special shipping requests have been made, our trained staff will send all orders by UPS Ground service. The appropriate shipping charges (freight & insurance costs) will be added to the invoice, unless otherwise instructed by the customer.

#### SPECIAL PRICING

We offer special pricing for volume purchases and standing orders. Please call a sales representative for more information on special pricing qualifications.

#### **RETURN POLICY**

Our Quality Manager will handle all returns. Before returning merchandise, please call to obtain a return authorization number from your sales representative. We will need to know the reason for the return, date of purchase, purchase order number and invoice number in order to issue a return authorization number. Returned merchandise must be received before a credit can be issued. Returns will not be accepted after 90 days. A restocking fee of 25% of the price paid, or a minimum of \$25.00 (whichever is greater) will be charged on all returns.

#### **WARRANTY**

All products manufactured by UCT are guaranteed against defects in materials and workmanship for a period of 90 days after shipment. UCT will replace any items that prove to be defective during this time period. The exclusive remedy requires the end user to first advise UCT of the defective product by phone or in writing and must include order number, the lot number and the shipping date.

To initiate this action, photographs of the product, including packaging and labeling of the containers, must be submitted to the UCT Representative for approval. With approval a return authorization can be initiated, and must be received within 30 days. Once the materials arrive at UCT a further inspection of the materials must be completed and accepted by our Quality Manager prior to further action of credits or replacement. UCT's total liability is limited to the replacement cost of UCT products.

This warranty does not apply to damage resulting from misuse.

#### **Contact Us**

Phone: 215.781.9255

UCT,Inc. 800.385.3153

Fax: 215.785.1226 2731 Bartram Rd. Bristol, PA 19007

Email: info@unitedchem.com

Web: www.unitedchem.com

ENVIRONMENTAL PRODUCTS CATALOG

UCT, Inc. | 2731 Bartram Rd | Bristol, PA 19007 | USA **P**. 800.385.3153 | 215.781.9255 | **F**. 215.785.1226

### www.unitedchem.com

Feedback on our new catalogue? Let us know what you think: info@unitedchem.com









